	How to correct an ABOCK when done by same tech as TSX	Dept:	324311
Wake Forest Baptist Medical Center		**Dept Name:**	Blood Bank
		Effective Date:	
	BB.BBIS.1012	**Revised Date:**	
Name & Title: CLIA Laboratory Medical Director		**Contact:**	Julie H. Simmons / Christina S. Warren
Signature: _69 Booper_		**Date:**	11/16/2020

1. General Procedure Statement:

A. **Purpose:** The purpose is to be able to perform an electronic crossmatch when the same person who resulted the type and screen test also resulted the ABOCK. Usually this is done when a type and screen is run on the instrument and resulted manually in SCC when the results do not cross from the instrument and that same tech performs and results the ABOCK.

B. **Responsible Department/Scope:**

   i. Procedure owner/Implementer: Julie H. Simmons/ Christina S. Warren
   ii. Procedure prepared by: Julie Jackson
   iii. Who performs procedure: Department staff/management

C. **Definitions:**

   TSX: SCC code for Type and Screen test
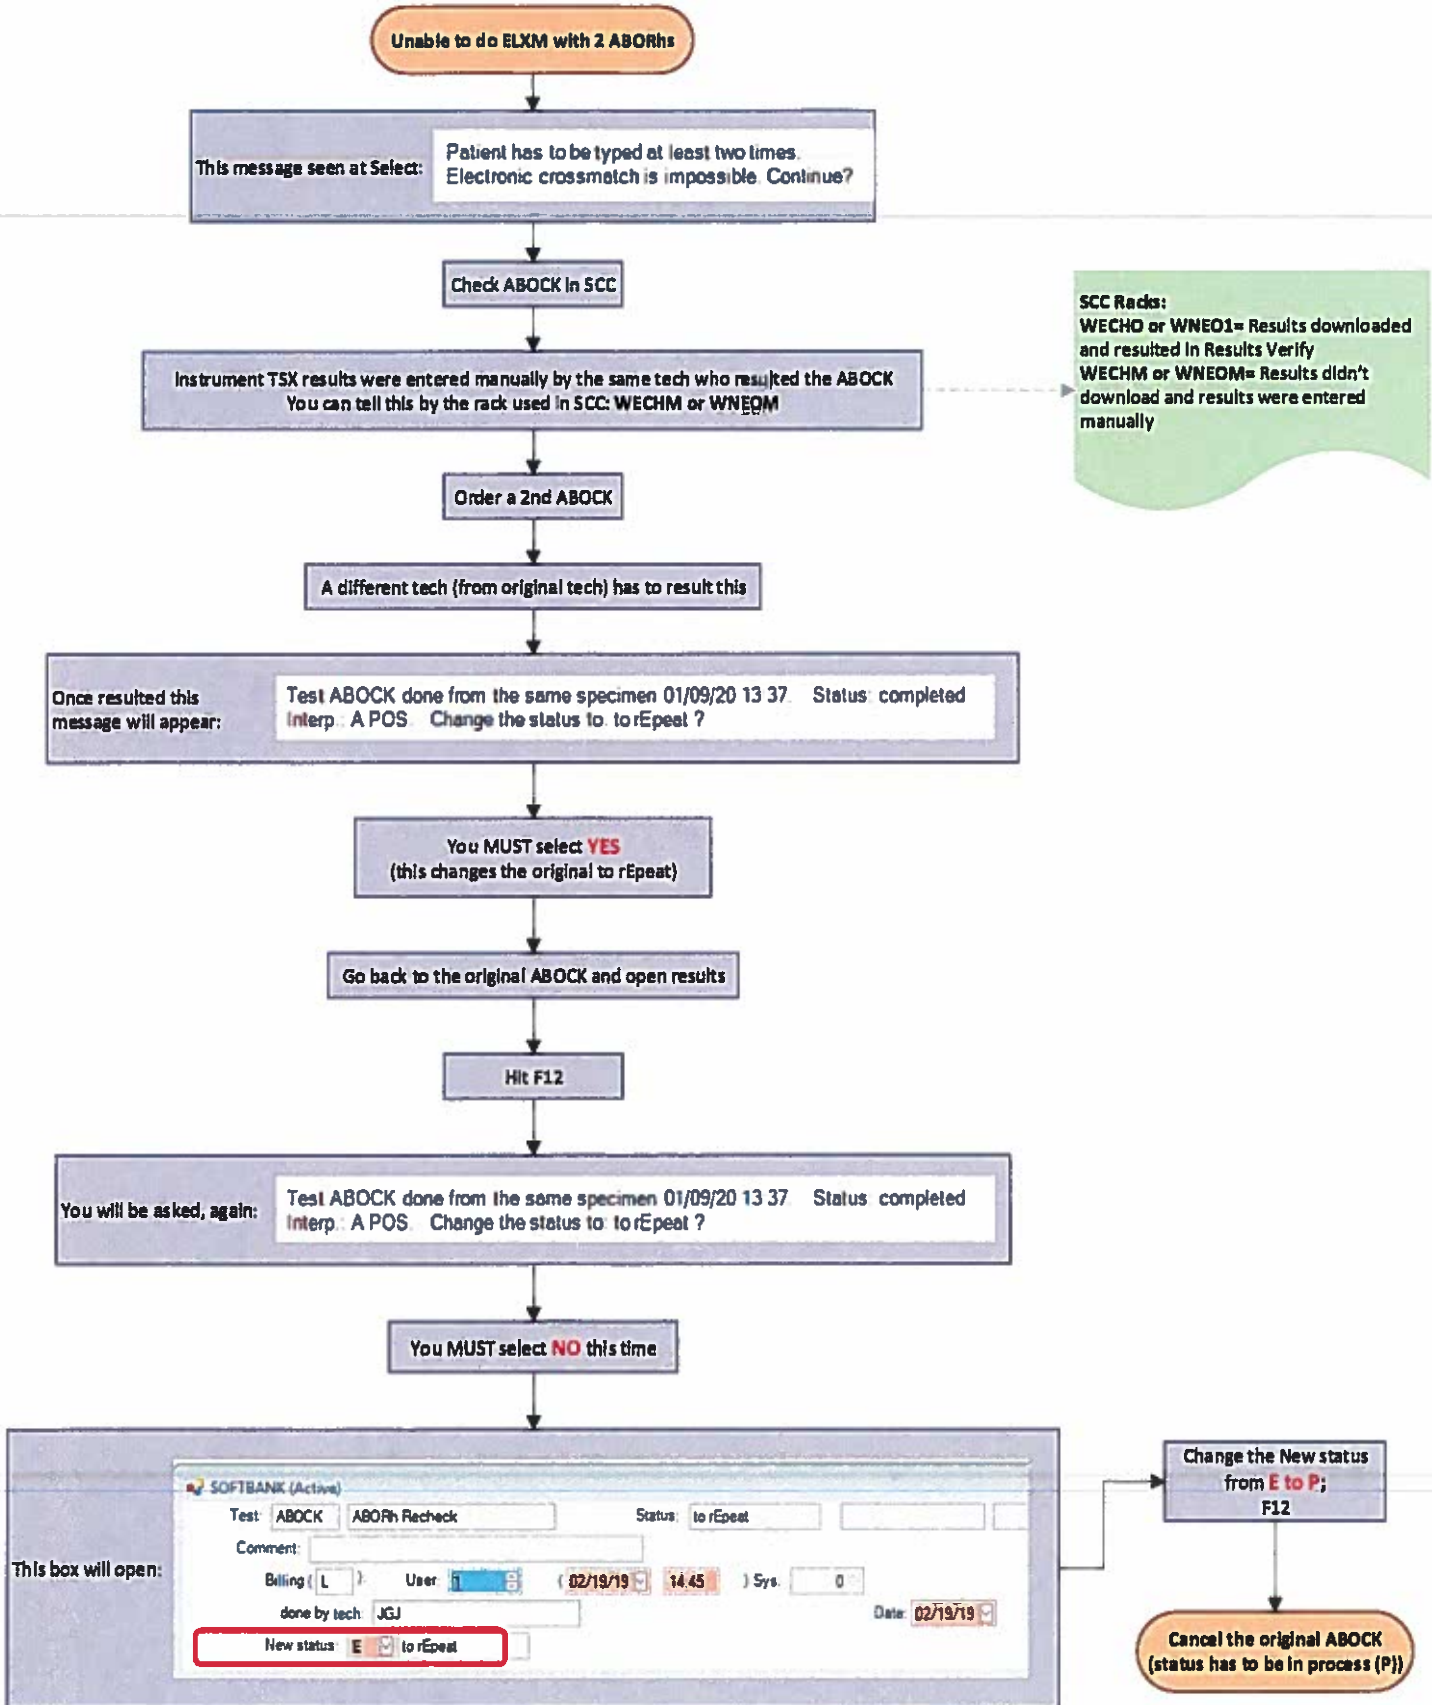
   ELXM: SCC code for Electronic crossmatch

   ABOCK: SCC code for ABORh recheck

   SCC: Blood Bank computer system, Soft Computer Company

D. **Sections:**
   NA

2. Procedure: HOW TO FIX ABOCK IN SCC WHEN SAME TECH RESULTS BOTH TSX AND ABOCK

Unable to do ELXM with 2 ABORhs

This message seen at Select:	Patient has to be typed at least two times. Electronic crossmatch is impossible. Continue?

Check ABOCK in SCC

Instrument TSX results were entered manually by the same tech who resulted the ABOCK You can tell this by the rack used in SCC: WECHM or WNEOM	SCC Racks: WECHO or WNEO1= Results downloaded and resulted In Results Verify WECHM or WNEOM= Results didn't download and results were entered manually

Order a 2nd ABOCK

A different tech (from original tech) has to result this

Once resulted this message will appear:	Test ABOCK done from the same specimen 01/09/20 13 37 Status: completed Interp.: A POS Change the status to: to rEpeat ?

You MUST select YES (this changes the original to rEpeat)

Go back to the original ABOCK and open results

Hit F12

You will be asked, again:	Test ABOCK done from the same specimen 01/09/20 13 37 Status: completed Interp.: A POS Change the status to: to rEpeat ?

You MUST select NO this time

This box will open:	**SOFTBANK (Active)** Test: ABOCK ABORh Recheck Status: to rEpeat Comment: Billing (L) User: 1 (02/19/19) 14.45) Sys. 0 done by tech JGJ Date: 02/19/19 New status E to rEpeat	**Change the New status from E to P; F12**

Cancel the original ABOCK (status has to be in process (P))

3. Review/Revised/Implemented:

All procedures must be reviewed according to the Document Change Protocol.
All new procedures that have major revisions must be signed by the CLIA Director.
All reviewed procedures with minor revisions can be signed by the designated section Medical Director.

4. Related Procedures:

NA

5. References:

NA

6. Attachments:

NA

7. Revised/Reviewed Dates and Signatures:

See Document Change Control

Document Change Control								

Title: How to correct an ABOCK when done by same tech as TSX

Previous title:								
Written date		1/9/20			Written by		JJackson	
Validation date		1/10/202~			Validation by		_(signature)_	
Reviewed date		1-16-2020			Reviewed by		_(signature)_	
Approved date		1/13/20			Approved by			
Approved date					Approved by			
Effective date in use		1-21-20			In use by		_(signature)_	

Revisions

Revised Date	By	MD Date	By	MD Date	By	Review Date	By	Effective Date	By

Validate Date	By	Revisions:							

Revised Date	By	MD Date	By	MD Date	By	Review Date	By	Effective Date	By

Validate Date	By	Revisions:							

Revised Date	By	MD Date	By	MD Date	By	Review Date	By	Effective Date	By

Validate Date	By	Revisions:							

Revised Date	By	MD Date	By	MD Date	By	Review Date	By	Effective Date	By

Validate Date	By	Revisions:							

Locations	BBIS Office Manual		Out of Use Date			By	
			Reason:				

Reviews: Record Date/Initials

Date	Initials	Date	Initials	Date	Initials	Date	Initials