

PROGRAM Standard Operating Procedure – Laboratory Services	
Title: MIC52400 – MAST Test	Policy Number:
Program Name: Laboratory Services	
Applicable Domain: Lab, DI and Pharmacy Services	
Additional Domain(s):	
Effective Date:	Next Review Date:
Issuing Authority: Director of Health Services	Date Approved:
Accreditation Canada Applicable Standard: N/A	

GUIDING PRINCIPLE:

The MAST test is used to detect AmpC and/or Extended Spectrum Beta-Lactamase enzyme production in Gram-negative bacilli.

PURPOSE/RATIONALE:

This standard operating procedure describes how to perform the MAST test.

SCOPE/APPLICABILITY:

This procedure applies to Medical Laboratory Technologists (MLTs) performing the MAST test.

SAMPLE INFORMATION:

Type	Few, well isolated colonies
-------------	-----------------------------

REAGENTS and/or MEDIA:

Type	MASTDISKS Combi AmpC and Extended Spectrum Beta-Lactamase (ESBL) Detection Disks: A = Cefpodoxime (10 ug) B = Cefpodoxime (10ug) + ESBL inhibitor C = Cefpodoxime (10ug) + AmpC inhibitor D = Cefpodoxime (10ug) + ESBL inhibitor + AmpC Inhibitor
Stability and Storage Requirements	<ul style="list-style-type: none"> Store at 2°C to 8°C in the container provided until the expiry date shown on the pack label Allow to equilibrate to room temperature before opening

Disclaimer Message: This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

SUPPLIES:

- Plastic Vitek tubes and caps
- Sterile saline
- Sterile swabs
- Mueller Hinton agar
- Forceps
- Small, metric ruler

EQUIPMENT

- DensiCHEK Plus
- 35° ambient air incubator

SPECIAL SAFETY PRECAUTIONS:

Containment Level 2 facilities, equipment, and operational practices for work involving infectious or potential infectious materials or cultures.

- Ensure that appropriate hand hygiene practices be used.
- Lab gown must be worn when performing activities with potential pathogens.
- Gloves must be worn when direct skin contact with infected materials is unavoidable.
- Eye protection must be used when there is a known or potential risk of exposure of splashes.
- All procedures that may produce aerosols, or involve high concentrations or large volumes should be conducted in a biological safety cabinet (BSC).
- The use of needles, syringes and other sharp objects should be strictly limited.

All patient specimens are assumed to be potentially infectious. Routine Practices must be followed. Since viable micro-organisms are used, all cultures must be handled with appropriate precautions. All equipment in contact with cultures should be decontaminated by appropriate methods.

QUALITY CONTROL:

- Quality control is performed weekly:
 - Positive: *Klebsiella pneumoniae* ATCC 700603, ESBL positive
 - Negative: *Escherichia coli* ATCC 25922, ESBL and AmpC negative
- A TQC order is automatically generated on Wednesdays to record the QC results

PROCEDURE INSTRUCTIONS:

Step	Action
Performing the MAST test	
1	Remove the MAST disks from refrigerator for 1 hour and bring to room temperature before opening the container.
2	Remove Mueller Hinton agar from the refrigerator and bring to room temperature.

Disclaimer Message: This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

3	Dispense 3 mL of sterile saline into a labelled plastic test tube. Pick several colonies from a fresh agar plate and prepare a suspension equivalent to a 0.5 McFarland standard.
4	Within 15 minutes of adjusting turbidity, dip a sterile cotton swab into the inoculum and rotate against the wall of the tube above the liquid to remove excess inoculum.
5	Swab the entire surface of the agar three times, rotating plate approximately 60° between streaking to ensure even distribution. To minimize aerosols, avoid hitting the sides of the plate. Finally, run swab around the edge of the agar to remove any excess moisture. Allow inoculated plate to stand for 3 to 15 minutes before applying disks.
6	Using sterile forceps, place one of each type of MAST disk onto the inoculated plate, ensuring sufficient space between the disks to allow formation of clearly defined zones of inhibition.
7	Invert the plate and incubate in the O ₂ incubator for 18 to 24 hours.
8	After incubation, read plates only if lawn of growth is confluent.
9	Use a ruler held on the back of the plate to measure and record in mm the diameter of any zones of inhibition that are observed. Disks showing no zone of inhibition should be recorded as 6mm.

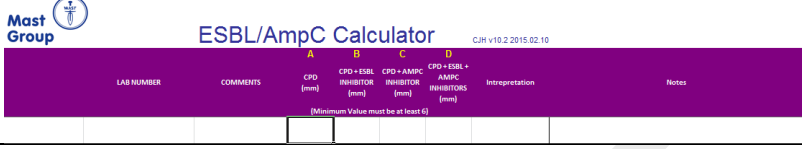
INTERPRETATION OF RESULTS:

1. Manual Interpretation:

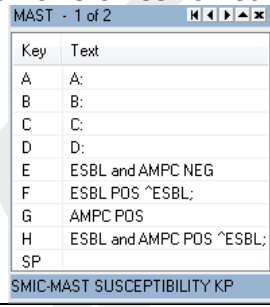
Step	Action
1	Compare the zone of inhibition of the Cefpodoxime disk (A) to the zones of inhibition of each the Cefpodoxime plus inhibitor disks (B, C & D)
	IF
	All zones are within 2 mm of each other
	THEN
	Organism is negative for both ESBL and AmpC activity
	IF
	Each of B - A and D - C is ≥5 mm AND the difference in zone diameter between disks B and D and A and C are ≤4 mm
THEN	
The organism is demonstrating ESBL activity and not AmpC activity	
IF	
Each of D - B and C - A is ≥5 mm AND the difference in zone diameter between disks A and B and disks C and D are ≤4 mm	
THEN	
The organism is demonstrating AmpC activity alone	
IF	
D-C is ≥5 mm AND the difference in zone diameter between disks A and B is ≤4 mm	
THEN	
The organism is demonstrating ESBL and AmpC combined activity	

Disclaimer Message: This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

2. Template interpretation:

Step	Action
1	<p>Open up the ESBL calculator program: I:drive: Stanton Hospital Share → LAB → Microbiology → ESBL worksheet → ESBL Calculator Spreadsheet</p> 
2	Input the zone sizes for the A, B, C and D disks.
3	The worksheet will calculate and interpret the results.

REPORTING INSTRUCTIONS:

Step	Action
1	<p>The MAST keypad allows the zone sizes for each disk to be recorded:</p> 
2	Enter in all the zone sizes and select the correct interpretation from the keypad based on the results from the worksheet.
3	If the isolate is ESBL positive, a new isolate will be created by the LIS and called "ESBL confirmed". This isolate is for epidemiology reporting and should not appear on the final report. Change the isolate number from 2 to an A to prevent it from reporting.

LIMITATIONS:

1. To avoid potentially erroneous results, do not test cartridges from different batches together, batches should never be mixed.
2. Organisms producing a fully resistant profile i.e. no zone of inhibition on all disks, could indicate demonstration of an M β L or KPC carbapenemase production, which could also be masking concurrent ESBL or AmpC expression.

REFERENCES:

1. MAST GROUP. (2018/02). *Combi AmpC and Extended Beta-Lactamase (ESBL) Detection Disks* package insert
2. CLSI. *Performance Standards for Antimicrobial Susceptibility Testing*. 31th ed. CLSI supplement M100. Wayne, PA: Clinical and Laboratory Standards Institute; 2021

Disclaimer Message: This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

APPROVAL:

Date

REVISION HISTORY:

REVISION	DATE	Description of Change	REQUESTED BY
1.0	04 Apr 19	Initial Release	L. Steven
2.0	30 Jun 21	Procedure reviewed and added to NTHSSA policy template	L. Steven

DRAFT

Disclaimer Message: This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.