Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

PROGRAM Standard Operating Procedure – Laboratory Services	
Title: MIC10100 -	Policy Number: 15-146-V1
Microbiology Specimen Processing	
Program Name: Laboratory Services	
Applicable Domain: Lab, DI and Pharmacy Services	
Additional Domain(s): NA	
Effective Date: 15/03/2024	Next Review Date: 15/03/2026
Issuing Authority:	Date Approved:
Director, Laboratory and Diagnostic Imaging Services	15/03/2024
Accreditation Canada Applicable Standard: NA	

#### **Uncontrolled When Printed**

#### **GUIDING PRINCIPLE:**

A guide to the processing of specimens submitted for bacterial culture for the following specimens:

- 1. Bacterial Vaginosis Screen...pg.3
- 2. Blood Culture:
  - a. Receiving Blood Culture bottles...pg.4
  - b. Positive Blood Culture in BACTEC FX...pq.6
  - c. Blood Culture received >24 hr...pg.8
- 3. Blood Product Culture...pg.11
- 4. Body Fluid Culture:
  - a. FLD received in sterile container...pg.12
  - b. FLD received in BC bottles <24 hr...pg.14
  - c. FLD received in BC bottles >24 hr...pq.16
- 5. CSF Culture...pg.19
- 6. Ear Culture...pg.20
- 7. Eve Culture:
  - a. Superficial Eye...pg.21
  - b. Deep Eye...pg.22

- 8. Genital Culture
  - a. Lower Genital Tract...pg.23
  - b. Upper Genital Tract...pg.24
- 9. Gonorrhoeae Culture...pg.25
- 10.GBS Screen...pg.26
- 11.IUD Culture...pg.27
- 12.MRSA Screen...pg.28
- 13.MRO Screen...pg.28
- 14. Nose Culture...pg. 29
- 15.Oral Culture...pg.29
- 16.Respiratory Culture...pg.30
- 17. Throat Culture...pg. 31
- 18.Tip Culture...pg.31
- 19.Toxigenic *C.difficile...*pg.32
- 20. Trichomonas Rapid Test...pg. 32
- 21. Urine Culture...pg. 32
- 22.VRE Screen...pg.33
- 23.Wet Prep Screen...pg.33
- 24. Wound Culture:
  - a. Superficial Wound...pg.34
  - b. Deep Wound...pg.35
- 25.Yeast Culture...pg.36

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: 15-146-V1 Date Approved: 15/03/2024 Page 1 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1

Date Approved: 15/03/2024

#### **PURPOSE/RATIONALE:**

This standard operating procedure describes the specimen processing for microbiology specimens at Stanton Territorial Hospital.

### **SCOPE/APPLICABILITY:**

This standard operating procedure applies to Medical Laboratory Technologists (MLTs) processing specimens for microbiology culture.

# **REAGENTS and/or MEDIA:**

- Anaerobic KV agar (KV)
- Blood agar (BA)
- Brucella agar (BRU)
- Chocolate agar (CHO)
- Colistin-nalidixic acid agar (CNA)
- LIM broth (LIM)
- MacConkey agar (MAC)

- MRSASelect II agar (MRS)
- Sabouraud agar (SAB)
- StrepBSelect agar (GBS)
- Thayer Martin agar (TM)
- Thioglycollate broth (THIO)
- UriSelect 4 agar (URI)
- VRE*Select* agar (VRE)

#### **SUPPLIES:**

- Disposable 1 μL and 10 μL loops
- Disposable needles
- Glass microscope slides
- Ringed cytology slides
- Alcohol swabs
- Sterile pipettes

- Sterile swabs
- Anaerobic trays and jars
- Anaerobic indicators
- AnaeroGen packs
- AnaeroPouch packs
- Blood culture subculture vents

# **EQUIPMENT:**

- Biosafety cabinet
- 35° ambient air and 35° CO<sub>2</sub> incubators

#### **SPECIAL SAFETY PRECAUTIONS:**

Containment Level 2 facilities, equipment, and operational practices for work involving infectious or potentially infectious materials or cultures:

- Ensure that appropriate hand hygiene practices be used
- Lab gown must be worn when performing activities with potential pathogens
- Gloves must be worn when direct skin contact with infected materials is unavoidable
- Eye protection must be used when there is a known or potential risk of exposure of splashes
- All procedures that may produce aerosols, or involve high concentrations or large volumes should be conducted in a biological safety cabinet (BSC)
- The use of needles, syringes and other sharp objects should be strictly limited

All patient specimens are assumed to be potentially infectious. Routine Practices must be followed. Since viable micro-organisms are used, all cultures must be handled with appropriate precautions. All equipment in contact with cultures should be decontaminated by appropriate methods.

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 2 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1
Next Review Date: 15/03/2026 Date Approved: 15/03/2024

# **QUALITY CONTROL:**

• Refer to MIC60010-Microbiology Quality Control procedure

• Refer to MIC60040-Culture Media Quality Control procedure

# 1. PROCEDURE INSTRUCTIONS: BACTERIAL VAGINOSIS SCREEN

Step	Action
1	<ul> <li>Posterior vaginal vault or vaginal orifice</li> <li>Only performed on patients that are &gt;13 years of age</li> <li>If specimen is received on patient ≤13 years of age, process as a genital culture</li> <li>Refer to MIC10110-Vaginal Swab Processing Job Aid for other tests ordered on vaginal swabs</li> </ul>
2	Specimen should be stored at room temperature.
3	<ul> <li>Criteria for rejection:</li> <li>1. Unlabeled/mislabelled specimen</li> <li>2. Specimen container label does not match patient identification on requisition</li> <li>3. Duplicate specimens obtained with same collection method within 24 hours</li> </ul>
4	<ul> <li>Label the following media/slides:</li> <li>Label the frosted end of a glass microscope slide with the accession number, patient's last name and specimen type</li> </ul>
5	Make Gram stain smear. Refer to MIC10000-Microbiology Specimen Handling.
6	Gram stain slide. Refer to MIC20100-Gram Stain.

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 3 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

# 2. PROCEDURE INSTRUCTIONS: BLOOD CULTURE

a. <b>R</b>	eceiving Blood Culture bottles
Step	Action
1	<ul><li>Blood</li><li>Sterile fluid received in blood culture bottles</li></ul>
2	Specimen should be stored at room temperature.
3	<ul> <li>Criteria for rejection: <ol> <li>Unlabeled/mislabelled specimen</li> <li>Specimen container label does not match patient identification on requisition</li> <li>Broken/cracked bottle</li> <li>NOTE: If patient has been treated with antibiotics, blood culture specimens are considered irretrievable. Waiver of responsibility form SCM40110 needs to be filled out by the responsible nurse</li> <li>NOTE: Except for the above conditions, blood culture specimens are not rejected regardless of delayed transport, if received frozen or if bottles are expired. Ensure the appropriate specimen quality comments are attached to the specimen in OE and process blood culture specimen</li> </ol> </li> </ul>
4	Blood culture bottles need to be collected and received into SoftMic before loaded onto the BACTEC FX analyzer. It is important when receiving blood culture bottles that they are received but <b>NOT</b> plated. The instrument will not issue preliminary and final no growth reports if the specimen has been plated.
5	Receiving can be performed in Order Entry:  1. Order blood culture bottles  2. Collect and receive bottles by selecting the Add button beside  Collected by and Received by:  CRBAE CXBAN  Source, BLOOD   MS   at   1154   2023-09-26     Add (F6)   Received by   MS   at   1154   2023-09-26     Add (F6)   Received by   MS   at   1154   2023-09-26     Add (F6)   Collected by   MS   at   1154   2023-09-26     Add (F6)   Coll

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

6

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

Receiving of multiple bottles can be performed in the Receiving Worklist:

- 1. Select **Receiving Worklist** icon on the main menu
- 2. Select Not Received:



3. Scan the blood culture bottles that you want to receive. Each bottle that has been scanned will have a red check mark beside the order on the left side:




4. Select **Setup/Label** from the menu on the right-hand side:



5. Ensure that **Specimen Received** is selected:



Ensure that Specimen Plated is NOT selected:




- 7. Once you have ensured that Specimen Received is selected, select the OK button to receive the specimens
- 8. Load bottles onto the BACTEC FX analyzer as per MIC71000-BACTEC **FX Instrument**

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 5 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

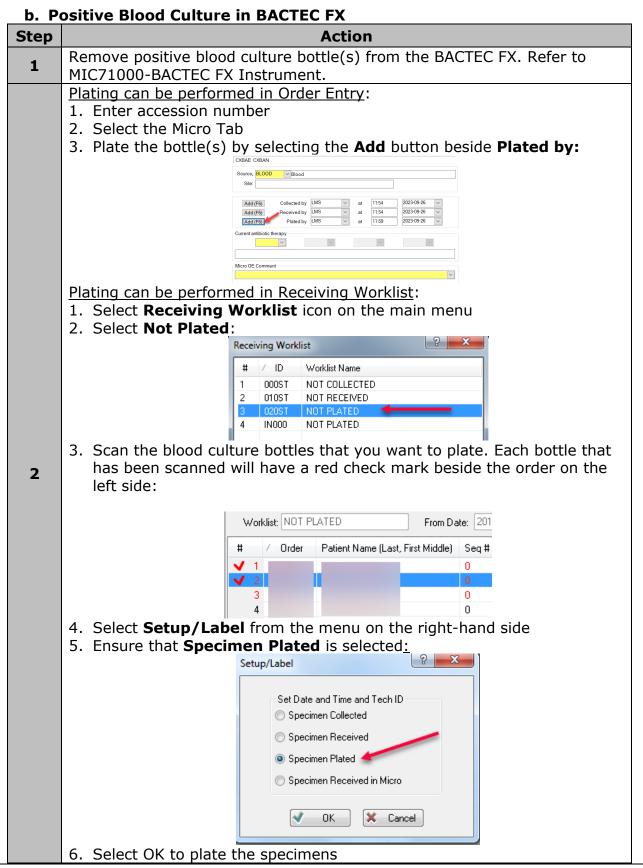

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 6 of 37 Type: Laboratory Services Program SOP

Title: MIC10100-Microbiology Specimen Processing Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

3	<ul> <li>Label the following media/slides:</li> <li>BA-C: Blood agar</li> <li>CHO-C: Chocolate agar</li> <li>MAC-O: MacConkey agar</li> <li>BRU-2: Brucella agar</li> <li>Label the frosted end of a glass microscope slide with the accession number, patient's last name, bottle type (AE/AN/PED)</li> <li>Clean slide with alcohol swab prior to inoculation</li> <li>NOTE: Indicate which bottle is positive on ALL plates and slides</li> </ul>
	NOTE: Indicate which bottle is positive on ALL plates and sides  NOTE: Indicate the date the bottle(s) went positive on all plates
4	<ol> <li>Working in the biosafety cabinet subculture the bottle(s):</li> <li>Swab the rubber septum with an alcohol pad and insert a vent</li> <li>Holding the bottle horizontally, place one drop on each plate and two small drops on the slide:</li> <li>Carefully pull the vent out of the bottle and discard it into the sharps container in the biosafety cabinet</li> <li>Using a sterile loop, streak the plates for isolation</li> <li>Spread the drop out on the FULL slide using the sterile loop:</li> </ol>
5	Place MAC plate in the O <sub>2</sub> incubator in white tray labeled "Positive Blood Culture."
6	Place BA and CHO plates in the CO <sub>2</sub> incubator in white tray labeled "Positive Blood Culture."
7	Place BRU in anaerobic jar or tray with anaerobic pouch and indicator as soon as practical after inoculation. Label jar or tray with date of 48 hour read. Anaerobes should not be exposed to air for 42-48 hours after inoculation. Refer to MIC10000-Microbiology Specimen Handling.
8	Gram stain slide. Refer to MIC20100-Gram Stain.  NOTE: Positive blood culture gram stains should be read within 1 hour of processing during regular Microbiology hours


Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 7 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024


### c. Blood Culture received >24 hr

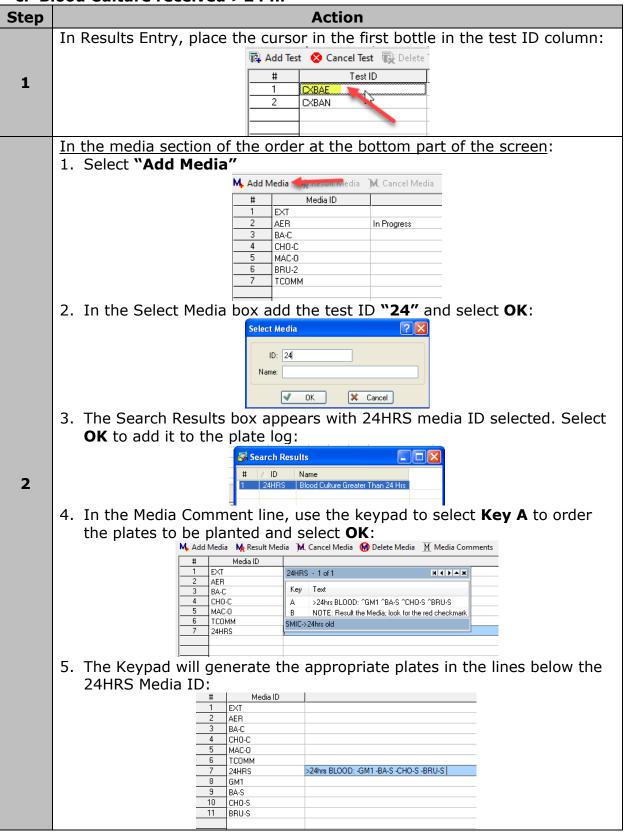

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

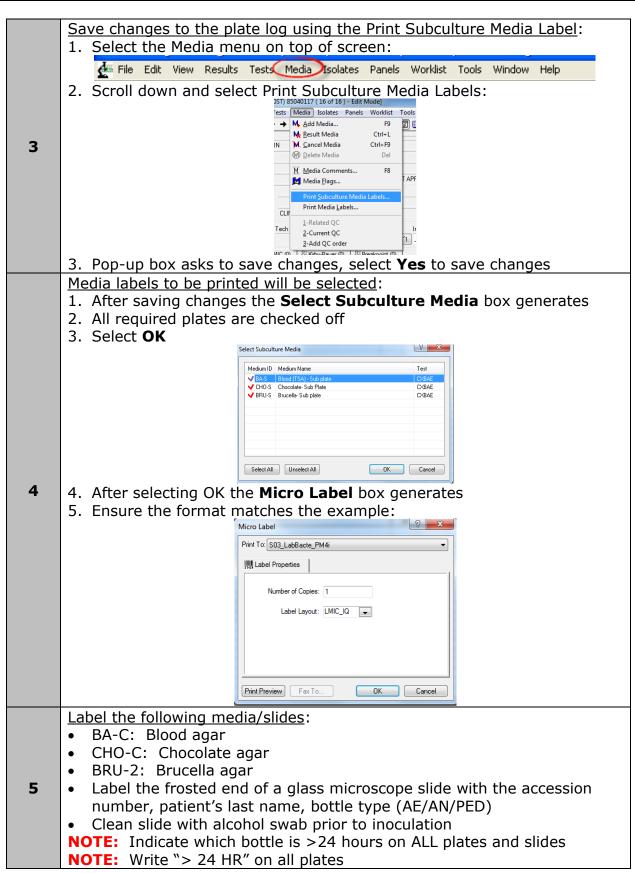

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 9 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1
Next Review Date: 15/03/2026 Date Approved: 15/03/2024

Working in the biosafety cabinet subculture the bottle(s): 1. Swab the rubber septum with an alcohol pad. Insert a vent into the bottle 2. Holding the bottle horizontally, place one drop on each plate and two small drops on the slide: 6 3. Carefully pull the vent out of the bottle and discard it into the sharps container in the biosafety cabinet 4. Using a sterile loop, streak the plates for isolation 5. Spread the drop out on the FULL slide using the sterile loop: Load bottles onto the BACTEC FX analyzer as per MIC71000-BACTEC FX 7 Instrument. Place BA and CHO plates in the CO<sub>2</sub> incubator in white tray labeled 8 "> 24 hr Blood Culture". Place BRU in anaerobic jar or tray with anaerobic pouch and indicator as soon as practical after inoculation. Label jar or tray with date of 48 hour 9 read. Anaerobes should not be exposed to air for 42-48 hours after inoculation. Refer to MIC10000-Microbiology Specimen Handling.

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Gram stain slide. Refer to MIC20100-Gram Stain.

10

Policy Number: Date Approved: Page 10 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

# 3. PROCEDURE INSTRUCTIONS: BLOOD PRODUCT CULTURE

		CEDURE INSTRUCTIONS: BLOOD PRODUCT CULTURE
S	Step	Action
	1	<ul> <li>Blood products need to be processed as:</li> <li>Body fluid culture received in blood culture bottles:</li> <li>CXFBC → Source → Blood product</li> <li>Body fluid culture:</li> <li>CXFLD → Source → Blood product</li> </ul>
	2	Specimen should be refrigerated.
	3	<ul><li><u>Criteria for rejection</u>:</li><li>1. Improperly collected, labeled, transported or handled specimens should be processed. Waiver of responsibility form SCM40110 needs to be filled out by the responsible nurse.</li></ul>
	4	<ol> <li>Processing CXFBC:</li> <li>20 mL of blood product is needed for the inoculation of blood culture bottles and 5 mL of blood product is needed for the inoculation of the body fluid culture media. If sufficient volume is received, proceed to step 3. If sufficient volume is not received, aseptically inject 10 to 20 mL of Thioglycollate broth into the blood product bag and mix.</li> <li>On the blood culture bottles, place a mark at 10 mL above the level of the broth. Remove the caps and clean the septum with an alcohol pad. Label bottles with LIS labels.</li> <li>Inspect the blood product bag and tubing and determine where the material will be taken from. Use alcohol pad to clean the area where the needle will be inserted.</li> <li>Using a butterfly needle and a vacutainer barrel, aseptically insert the needle end into the blood product bag. Using the barrel, attach a blood culture bottle and fill to the 10 mL mark. Repeat with the second bottle. Also collect a red top vacutainer tube.</li> <li>Remove the butterfly needle from the blood product and dispose of carefully into the sharps container. Place a piece of tape over the hole and place the blood product bag into a large biohazard bag and store in refrigerator until testing is complete.</li> <li>Load bottles onto the BACTEC FX analyzer as per MIC71000-BACTEC FX Instrument.</li> </ol>
	5	<ol> <li>Processing CXFLD:</li> <li>From the red top tube collected above, use a sterile pipette to inoculate Blood agar, Chocolate agar and Brucella agar and make a gram stain with one drop of the blood product. Streak out to cover whole plate.</li> <li>Place BA and CHO plates in the CO<sub>2</sub> incubator on "New Wound Culture" shelf.</li> <li>Place BRU in anaerobic jar or tray with anaerobic pouch and indicator as soon as practical after inoculation. Label jar or tray with date of 48 hour read. Anaerobes should not be exposed to air for 42-48 hours after inoculation. Refer to MIC10000-Microbiology Specimen Handling.</li> <li>Gram stain slide. Refer to MIC20100-Gram Stain.</li> <li>NOTE: Gram stain must be read before culture plates</li> </ol>

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 11 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1

Next Review Date: 15/03/2026

Policy Number: 15-146-V1

Date Approved: 15/03/2024

4. PROCEDURE INSTRUCTIONS: BODY FLUID CULTURE

	ody fluid received in sterile container:
Step	Action
_	<ul> <li>Fluid should be collected in a sterile specimen container or tube and/or into blood culture bottles</li> <li>If fluid is received in blood culture bottles, refer to part b.</li> </ul>
1	<ul> <li>If swab is received, add Specimen Quality comment SWBFL</li> <li>Refer prosthetic device specimens for culture to <i>Dyna</i>LIFE</li> <li>Refer tissue or biopsy specimens for culture to <i>Dyna</i>LIFE</li> </ul>
2	Specimen should be stored at room temperature.  NOTE: If a delay in processing is anticipated, do NOT refrigerate
3	<ol> <li>Criteria for rejection:         <ol> <li>Insufficient volume for tests requested: contact the physician to prioritize requests</li> <li>Leaking specimens should be processed, but alert the physician of the possibility of contamination</li> <li>Specimens received in the laboratory in a syringe with the needle still attached will be rejected. In addition, an RL6 will be filed outlining the hazard. Refer to SCM40100-Specimen Acceptance and Rejection Policy</li> <li>Improperly collected, labeled, transported or handled specimens should be processed. Waiver of responsibility form SCM40110 needs to be filled out by the responsible nurse</li> <li>If only blood culture bottles are received, a gram stain cannot be performed</li> </ol> </li> </ol>
4	<ul> <li>Volume received: (Tube 2 is the usual tube for Microbiology)</li> <li>&gt;1mL: Centrifuge at 3500 rpm for 10 minutes (Program 2). Remove supernatant with sterile pipette and place into red top tube labeled with SUP label. Mix sediment with pipette.</li> <li>&lt;=1mL: Inoculate plates using a sterile pipette.</li> <li>NOTE: If sample is NOT centrifuged, add Specimen Quality comment NOSPI to state: "Sample not concentrated"</li> </ul>
5	<ul> <li>Label the following media/slides:</li> <li>BA-C: Blood agar</li> <li>CHO-C: Chocolate agar</li> <li>MAC-O: MacConkey agar</li> <li>BRU-2: Brucella agar</li> <li>THIO2: Thioglycollate broth</li> <li>Label the frosted end of a microscope slide with the accession number, patient's last name and specimen type. Clean slide with alcohol swab prior to inoculation</li> </ul>
6	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.
7	Make Gram stain smear. Refer to MIC10000-Microbiology Specimen Handling.
8	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.
9	Place MAC plate in the O <sub>2</sub> incubator on "New Wound Culture" shelf.

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 12 of 37

Type: Laboratory Services Program SOP

Title: MIC10100-Microbiology Specimen Processing Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

10	Place BA and CHO plates in the CO <sub>2</sub> incubator on "New Wound Culture" shelf.
11	Place BRU in anaerobic jar or tray with anaerobic pouch and indicator as soon as practical after inoculation. Label jar or tray with date of 48 hour read. Anaerobes should not be exposed to air for 42-48 hours after inoculation. Refer to MIC10000-Microbiology Specimen Handling.
12	Label THIO with Day 2 date and Day 5 date. Place THIO broth in THIO rack in O <sub>2</sub> incubator in "Day 2" row.  NOTE: If fluid is from above the neck, keep THIO and BRU for 10 days
13	Gram stain slide. Refer to MIC20100-Gram Stain.  NOTE: Fluid gram stains should be read within 1 hour of processing during regular Microbiology laboratory hours

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 13 of 37 Title: MIC10100-Microbiology Specimen Processing Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Type: Laboratory Services Program SOP

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

<u>b. B</u>	ody fluid received in blood culture bottle <24 hours old:
Step	Action
1	Sterile fluid received in blood culture bottles
2	Specimen should be stored at room temperature.
3	<ul> <li>Criteria for rejection: <ol> <li>Unlabeled/mislabelled specimen</li> <li>Specimen container label does not match patient identification on requisition</li> <li>Broken/cracked bottle</li> <li>NOTE: If patient has been treated with antibiotics, fluid specimens in blood culture bottles are considered irretrievable. Waiver of responsibility form SCM40110 needs to be filled out by the responsible nurse</li> <li>NOTE: Except for the above conditions, fluid specimens in blood culture bottles are not rejected regardless of delayed transport, if received frozen or if bottles are expired. Ensure the appropriate specimen quality comments are attached to the specimen in OE and process blood culture specimen</li> </ol> </li> </ul>
4	Sterile body fluids received in blood culture bottles need to be collected and received into SoftMic before loaded onto the BACTEC FX analyzer. It is important when receiving sterile body fluids blood culture bottles that they are received but <b>NOT</b> plated. The instrument will not issue preliminary and final no growth reports if the specimen has been plated.
5	Receiving can be performed in Order Entry:  1. Order sterile body fluid received in blood culture bottles as CXFBC  2. Collect and receive bottles by selecting the Add button beside  Collected by and Received by:    CXEAR CYBAN   Source   BLOOD   Blood

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

6

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

Receiving of multiple bottles can be performed in the Receiving Worklist:

- 1. Select **Receiving Worklist** icon on the main menu
- 2. Select Not Received:



3. Scan the blood culture bottles that you want to receive. Each bottle that has been scanned will have a red check mark beside the order on the left side:




4. Select **Setup/Label** from the menu on the right-hand side:



5. Ensure that **Specimen Received** is selected:



Ensure that Specimen Plated is NOT selected:




- 7. Once you have ensured that Specimen Received is selected, select the OK button to receive the specimens
- 8. Load bottles onto the BACTEC FX analyzer as per MIC71000-BACTEC **FX Instrument**

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 15 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024


c. Body fluid received in blood culture bottle >24 hours old:

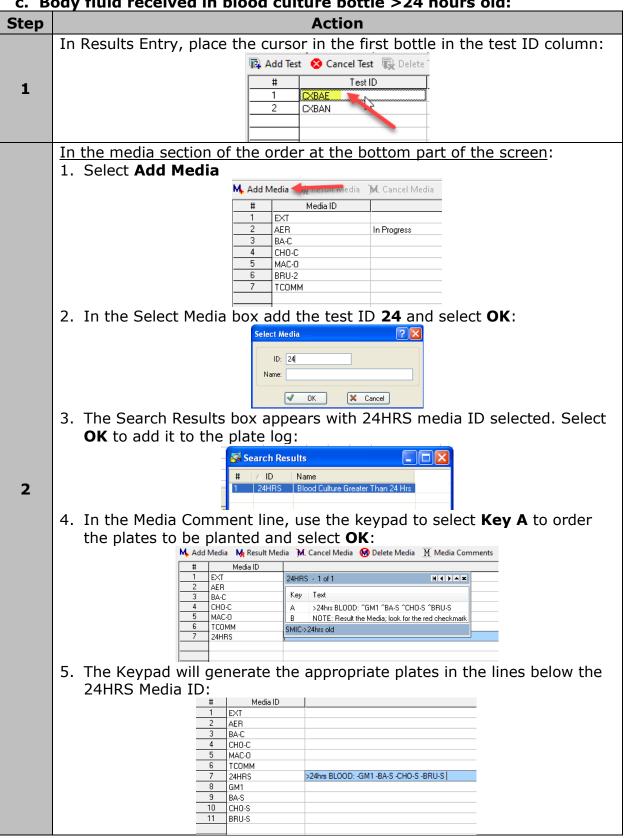

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

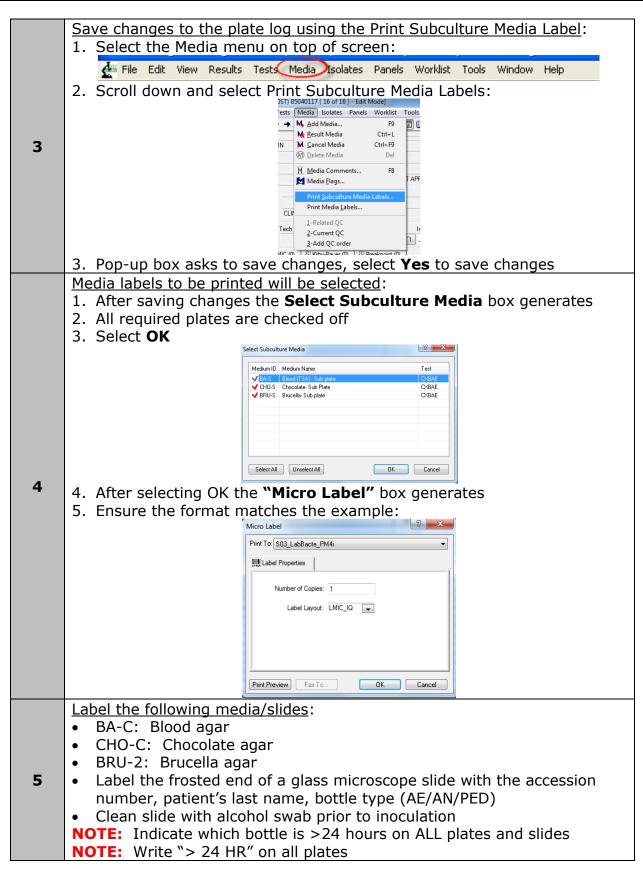

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 17 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1
Next Review Date: 15/03/2026 Date Approved: 15/03/2024

Working in the biosafety cabinet subculture the bottle(s): 1. Swab the rubber septum with an alcohol pad. Insert a vent into the bottle 2. Holding the bottle horizontally, place one drop on each plate and two small drops on the slide: 6 3. Carefully pull the vent out of the bottle and discard it into the sharps container in the biosafety cabinet 4. Using a sterile loop, streak the plates for isolation 5. Spread the drop out on the FULL slide using the sterile loop: Load bottles onto the BACTEC FX analyzer as per MIC71000-BACTEC FX 7 Instrument. Place BA and CHO plates in the CO<sub>2</sub> incubator in white tray labeled 8 "> 24 hr Blood Culture". Place BRU in anaerobic jar or tray with anaerobic pouch and indicator as soon as practical after inoculation. Label jar or tray with date of 48 hour 9 read. Anaerobes should not be exposed to air for 42-48 hours after inoculation. Refer to MIC10000-Microbiology Specimen Handling. 10 Gram stain slide. Refer to MIC20100-Gram Stain.

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 18 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

# 5. PROCEDURE INSTRUCTIONS: CSF CULTURE

Step	Action
1	Central nervous system shunt fluid
_	CSF from lumbar puncture
2	Specimen should be stored at room temperature.
_	NOTE: If a delay in processing is anticipated, do NOT refrigerate
3	<ol> <li>Criteria for rejection:</li> <li>Insufficient volume for tests requested: contact the physician to prioritize requests</li> <li>Leaking specimens should be processed, but alert the physician of the possibility of contamination</li> <li>Improperly collected, labeled, transported or handled specimens should be processed. Waiver of responsibility form SCM40110 needs to be filled out by the responsible nurse</li> </ol>
4	<ul> <li>Volume received: (Tube 2 is the usual tube for Microbiology)</li> <li>&gt;1mL: Centrifuge at 3500 rpm for 10 minutes (Program 2). Remove supernatant with sterile pipette and place into red top tube labeled with SUP label. Mix sediment with pipette</li> <li>&lt;=1mL: Inoculate plates using a sterile pipette</li> </ul>
5	<ul> <li>Label the following media/slides:</li> <li>BA-C: Blood agar</li> <li>CHO-C: Chocolate agar</li> <li>MAC-O: MacConkey agar</li> <li>Label the frosted end of a ringed cytology slide with the accession number, patient's last name and specimen type</li> <li>Clean slide with alcohol swab prior to inoculation</li> <li>NOTE: If specimen is from a shunt, THIO needs to be added</li> </ul>
6	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.
7	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.
8	Place the remaining sample sediment, supernatant in the $O_2$ incubator in sample bucket.
9	Place BA and CHO plates in the CO <sub>2</sub> incubator on "New Wound Culture" shelf.
10	Place MAC plate in the O <sub>2</sub> incubator on "New Wound Culture" shelf.
11	Gram stain slide. Refer to MIC20100-Gram Stain.  NOTE: CSF gram stains should be read within 1 hour of processing during regular Microbiology hours

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 19 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

# 6. PROCEDURE INSTRUCTIONS: EAR CULTURE

Step	Action
1	<ul> <li>External auditory canal (outer ear)</li> <li>Otitis media discharge swabbed from external auditory canal</li> <li>NOTE: Typanocentesis fluid should be ordered as a body fluid culture</li> </ul>
2	Specimen should be stored at room temperature.  NOTE: If transport is >2 hours, swabs should be refrigerated
3	<ul><li><u>Criteria for rejection</u>:</li><li>1. Unlabeled/mislabelled specimen</li><li>2. Specimen container label does not match patient identification on requisition</li></ul>
4	<ul> <li>Label the following media/slides:</li> <li>BA-C: Blood agar</li> <li>CHO-C: Chocolate agar</li> <li>CNA-C: Colistin-nalidixic acid agar</li> <li>MAC-O: MacConkey agar</li> <li>Label the frosted end of a glass microscope slide with the accession number, patient's last name and specimen type</li> </ul>
5	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.
6	Make Gram stain smear. Refer to MIC10000-Microbiology Specimen Handling.
7	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.
8	Place MAC plate in the $O_2$ incubator on "New Respiratory Culture" shelf.
9	Place BA, CHO and CNA plates in the CO <sub>2</sub> incubator on "New Respiratory Culture" shelf.
10	Gram stain slide. Refer to MIC20100-Gram Stain.

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 20 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

7. PROCEDURE INSTRUCTIONS: EYE CULTURE

a. Superficial Eye

Step	Action
1	<ul><li>Conjunctiva</li><li>Superficial corneal specimens</li></ul>
2	Specimen should be stored at room temperature.
3	<ul><li><u>Criteria for rejection</u>:</li><li>1. Unlabeled/mislabelled specimen</li><li>2. Specimen container label does not match patient identification on requisition</li></ul>
4	<ul> <li>Label the following media/slides:</li> <li>BA-C: Blood agar</li> <li>CHO-C: Chocolate agar</li> <li>Label the frosted end of a glass microscope slide with the accession number, patient's last name and specimen type</li> </ul>
5	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.
6	Make Gram stain smear. Refer to MIC10000-Microbiology Specimen Handling.
7	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.
8	Place BA and CHO plates in the CO <sub>2</sub> incubator on "New Respiratory Culture" shelf.
9	Gram stain slide. Refer to MIC20100-Gram Stain.

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 21 of 37 Type: Laboratory Services Program SOP

Title: MIC10100-Microbiology Specimen Processing Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

h. Deen Eve

	eep Eye
Step	Action
1	Corneal scrapings     Aguage (vitrage a fluid)
	<ul><li>Aqueous/vitreous fluid</li><li>Keratitis</li></ul>
2	Specimen should be stored at room temperature.
	·
	<u>Criteria for rejection</u> :  1. Unlabeled/mislabelled swabs
	Specimen container label does not match patient identification on
3	requisition
	3. Improperly collected, labeled, transported or handled specimens should
	be processed. Waiver of responsibility form SCM40110 needs to be
	filled out by the responsible nurse
	<u>Label the following media/slides</u> :  • BA-C: Blood agar
	CHO-C: Chocolate agar
	MAC-O: MacConkey agar
4	BRU-2: Brucella agar
	Label the frosted end of a glass microscope slide with the accession
	number, patient's last name and specimen type
	Clean slide with alcohol swab prior to inoculation
5	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen
	Handling.
6	Make Gram stain smear. Refer to MIC10000-Microbiology Specimen Handling.
_	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen
7	Handling.
8	Place MAC plate in the O <sub>2</sub> incubator on "New Respiratory Culture" shelf.
9	Place BA and CHO plates in the CO <sub>2</sub> incubator on "Respiratory Culture"
9	shelf.
	Place BRU in anaerobic jar or tray with anaerobic pouch and indicator as
10	soon as practical after inoculation. Label jar or tray with date of 48 hour
	read. Anaerobes should not be exposed to air for 42-48 hours after inoculation. Refer to MIC10000-Microbiology Specimen Handling.
	Gram stain slide. Refer to MIC20100-Microbiology Specimen Handling.
11	NOTE: Deep eye stains should be read within 1 hour of processing during
	regular Microbiology hours

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 22 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

# 8. PROCEDURE INSTRUCTIONS: GENITAL CULTURE

# a. Lower Genital Tract

Step	Action
1	<ul> <li>Cervix</li> <li>Labia</li> <li>Penis</li> <li>Vagina</li> <li>Vulva</li> </ul>
2	Specimen should be stored at room temperature.
3	<ol> <li>Criteria for rejection:         <ol> <li>Unlabeled/mislabelled specimen</li> <li>Specimen container label does not match patient identification on requisition</li> <li>Do not accept vaginal swabs from women &gt;13 years of age for genital culture unless significant clinical information is provided. Refer to MIC10231-Vaginal Swab Processing Job Aid</li> </ol> </li> <li>Do not process vaginal swabs for yeast culture unless significant clinical information is provided. Refer to MIC10110-Vaginal Swab Processing Job Aid</li> </ol>
4	<ul> <li>Label the following media/slides:</li> <li>BA-C: Blood agar</li> <li>CHO-C: Chocolate agar</li> <li>TM-C: Thayer Martin agar</li> <li>MAC-O: MacConkey agar</li> <li>Label the frosted end of a glass microscope slide with the accession number, patient's last name and specimen type</li> </ul>
5	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.
6	Make Gram stain smear. Refer to MIC10000-Microbiology Specimen Handling.
7	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.
8	Place MAC plate in the O <sub>2</sub> incubator on "New Urine Culture" shelf.
9	Place BA, CHO and TM plates in the CO <sub>2</sub> incubator on "New Urine Culture" shelf.
10	Gram stain slide. Refer to MIC20100-Gram Stain.

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 23 of 37 Title: MIC10100-Microbiology Specimen Processing Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Type: Laboratory Services Program SOP

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

<u>b. U</u>	b. Upper Genital Tract	
Step	Action	
1	<ul> <li>Endometrial swabs, biopsies and curettings</li> <li>Placenta swabs and tissues</li> <li>Products of conception, endometrial/uterine, Cul de Sac/transvaginal, fallopian tube, tubo-ovarian swabs or aspirates</li> </ul>	
2	Specimen should be stored at room temperature.	
3	<ul> <li>Criteria for rejection:</li> <li>1. Unlabeled/mislabelled specimen</li> <li>2. Specimen container label does not match patient identification on requisition</li> <li>3. Improperly collected, labeled, transported or handled irretrievable specimens should be processed. Waiver of responsibility form SCM40110 needs to be filled out by the responsible nurse</li> </ul>	
4	Label the following media/slides:  BA-C: Blood agar  CHO-C: Chocolate agar  TM-C: Thayer Martin agar  MAC-O: MacConkey agar  BRU-2: Brucella agar  THIO2: Thioglycollate broth  Label the frosted end of a glass microscope slide with the accession number, patient's last name and specimen type  Clean slide with alcohol swab prior to inoculation	
5	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.	
6	Make Gram stain smear. Refer to MIC10000-Microbiology Specimen Handling.	
7	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.	
8	Place MAC plate in the O₂ incubator on "New Urine Culture" shelf.	
9	Place BA, CHO and TM plates in the CO <sub>2</sub> incubator on "New Urine Culture" shelf.	
10	Place BRU in anaerobic jar or tray with anaerobic pouch and indicator as soon as practical after inoculation. Label jar or tray with date of 48 hour read. Anaerobes should not be exposed to air for 42-48 hours after inoculation. Refer to MIC10000-Microbiology Specimen Handling.	
11	Label THIO with Day 2 date and Day 5 date. Place THIO broth in THIO rack in $O_2$ incubator in "Day 2" row.	
12	Gram stain slide. Refer to MIC20100-Gram Stain.	

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 24 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1
Next Review Date: 15/03/2026 Policy Number: 15/03/2024

# 9. PROCEDURE INSTRUCTIONS: GONORRHOEAE CULTURE

	LEDURE INSTRUCTIONS: GONORRHOEAE CULTURE
Step	Action
1	<ul> <li>Urethra (male specimens only)</li> <li>Cervix</li> <li>Throat</li> <li>Eye</li> <li>Rectum</li> </ul>
2	Specimen can be stored at room temperature or refrigerated.
3	<ul><li>Criteria for rejection:</li><li>1. Unlabeled/mislabelled specimen</li><li>2. Specimen container label does not match patient identification on requisition</li></ul>
4	<ul> <li>Label the following media/slides:</li> <li>CHO-C: Chocolate agar</li> <li>TM-C: Thayer Martin agar</li> <li>If the source is urethra, label the frosted end of a glass microscope slide with the accession number, patient's last name and specimen type</li> <li>NOTE: Slides are only made on urethra specimens, not cervix, eye or throat</li> <li>NOTE: If gonorrhoeae culture is ordered on throat or eye specimens, full culture along with gonorrhoeae culture will be performed. In order entry, when ordering CXGON, if throat or eye is selected as the source, the throat culture or eye culture is automatically ordered</li> </ul>
5	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.
6	If applicable, make Gram stain smear. Refer to MIC10000-Microbiology Specimen Handling.
7	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.
8	Place CHO and TM plates in the CO <sub>2</sub> incubator on "New Urine Culture" shelf.
9	If applicable, gram stain slide. Refer to MIC20100-Gram Stain.

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 25 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1
Next Review Date: 15/03/2026 Policy Number: 15/03/2024

10. PROCEDURE INSTRUCTIONS: GBS SCREEN

	RUCEDURE INSTRUCTIONS: GBS SCREEN
Step	Action
1	<ul> <li>Vaginal-Rectal</li> <li>Specimen for GBS screening in pregnancy should be collected at 35 to 37 weeks gestation</li> </ul>
2	Specimen should be stored at room temperature.
3	<ul><li>Criteria for rejection:</li><li>1. Unlabeled/mislabelled specimen</li><li>2. Specimen container label does not match patient identification on requisition</li></ul>
4	Label the following media/slides:  • LIM-C: LIM broth  • GBS-O: StrepB Select agar  ➤ Attach the GBS-O label to the clip on the front of the BSC
5	Break the swab off into the LIM broth. Recap loosely.
6	<ul> <li>Incubate the media as follows:</li> <li>LIM Broth: CO₂ incubator</li> <li>This is done by the technologist performing daily shutdown duties</li> </ul>
7	<ul> <li>After 18-24hr incubation:</li> <li>Remove the required number of StrepB Select agar plates from the refrigerator and bring to room temperature</li> <li>Label the GBS-O plates with the labels clipped to the BSC</li> <li>Remove LIM broth from incubator and subculture to the GBS-O plates:</li> <li>Saturate a sterile swab in the broth and rotate against the wall of the tube above the liquid to remove excess inoculum and swab the first quadrant of the agar</li> <li>Streak for isolated growth using a disposable inoculation needle</li> <li>Streak out to cover the whole plate</li> </ul>
8	Place GBS plate in the O <sub>2</sub> incubator on "New Urine Culture" shelf.

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 26 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1
Next Review Date: 15/03/2026 Policy Number: 15/03/2024

# 11. PROCEDURE INSTRUCTIONS: IUD CULTURE

Step	Action
1	Specimen should be refrigerated.
2	<ul><li>Criteria for rejection:</li><li>1. Unlabeled/mislabeled specimen.</li><li>2. Specimen container label does not match patient identification on requisition.</li></ul>
3	<ul><li>Label the following media/slides:</li><li>THIO2: Thioglycollate broth</li><li>BRU-2: Brucella agar</li></ul>
4	Add a full tube of thioglycollate broth (not the labelled tube) to the specimen container containing the IUD and vortex for 30 seconds.
5	Using a sterile pipette, transfer the THIO broth into a red top vacutainer tube and centrifuge at 3500 rpm for 10 minutes.
6	After centrifugation is complete, using a STERILE pipette, dispense the fluid sediment as follows (discard supernatant in red top tube):  1 drop on BRU  2-5 drops in labelled Thioglycollate broth
7	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.
8	Label THIO with Day 2 date, Day 5 date and Day 10 date. Place THIO broth in THIO rack in $O_2$ incubator in "Day 2" row.
9	Place BRU in anaerobic jar or tray with anaerobic pouch and indicator as soon as practical after inoculation. Label jar or tray with date of 48 hour read. Anaerobes should not be exposed to air for 42-48 hours after inoculation. Refer to MIC10000-Microbiology Specimen Handling.
10	Gram stain is not performed. No slide is required.

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 27 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

#### **12.** PROCEDURE INSTRUCTIONS: MRSA SCREEN

Step	Action
NOTE	Due to incubation requirements, MRSA plates are set up until 15:00
1	<ul> <li>Bilateral nasal swab</li> <li>Bilateral groin swab</li> <li>Swab specimen from various sources</li> </ul>
2	Specimen should be stored at room temperature.
3	<ul> <li>Criteria for rejection:</li> <li>1. Unlabeled/mislabelled specimen</li> <li>2. Specimen container label does not match patient identification on requisition</li> <li>3. Duplicate specimens obtained with same collection method from same collection location within 24 hours</li> </ul>
4	<u>Label the following media/slides</u> : • MRS-O: MRSA <i>Select</i> II agar
5	Inoculate plate with specimen. Refer to MIC10000-Microbiology Specimen Handling.
6	Streak plate for isolation. Refer to MIC10000-Microbiology Specimen Handling.
7	Place MRS plate in the O <sub>2</sub> incubator on "New Urine Culture" shelf.

#### **13**. PROCEDURE INSTRUCTIONS: MRO SCREEN

Step	Action
NOTE	Due to incubation requirements, MRO plates are set up until 15:00
1	Swab specimen from various sources
2	Specimen should be stored at room temperature.
3	<ul> <li>Criteria for rejection:</li> <li>1. Unlabeled/mislabelled specimen</li> <li>2. Specimen container label does not match patient identification on requisition</li> <li>3. Duplicate specimens obtained with same collection method from same collection location within 24 hours</li> </ul>
4	<u>Label the following media/slides</u> :  • MRS-O: MRSA <i>Select</i> II agar  • VRE-O: VRE <i>Select</i> agar
5	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.
6	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.
7	Place MRS and VRE plates in the O <sub>2</sub> incubator on "New Urine Culture" shelf.

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 28 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1
Next Review Date: 15/03/2026 Date Approved: 15/03/2024

14. PROCEDURE INSTRUCTIONS: NASAL CULTURE

Step	Action
Step	Action
1	• Nose
2	Specimen should be stored at room temperature.
3	<ul><li>Criteria for rejection:</li><li>1. Unlabeled/mislabelled specimen</li><li>2. Specimen container label does not match patient identification on requisition</li></ul>
4	<u>Label the following media/slides</u> :  • BA-C: Blood agar
5	Inoculate plate with specimen. Refer to MIC10000-Microbiology Specimen Handling.
6	Streak plate for isolation. Refer to MIC10000-Microbiology Specimen Handling.
7	Place BA plate in the $CO_2$ incubator on "New Respiratory Culture" shelf.
8	Gram stain is not performed. No slide is required.

#### 15. PROCEDURE INSTRUCTIONS: ORAL CULTURE

	ROCEDURE INSTRUCTIONS. ORAL COLTORE
Step	Action
1	Mouth
	Tongue
2	Specimen should be stored at room temperature.
	<u>Criteria for rejection</u> :
3	Unlabeled/mislabelled specimen
	2. Specimen container label does not match patient identification on
	requisition
Λ	Label the following media/slides:
4	SAB-R: Sabouraud dextrose agar
5	Inoculate plate with specimen. Refer to MIC10000-Microbiology Specimen
3	Handling.
6	Streak plate for isolation. Refer to MIC10000-Microbiology Specimen
O	Handling.
7	Label SAB plate with R: (Date + 2 date).
8	Place SAB plate on urine bench and "incubate" at room temperature.
9	Gram stain is not performed. No slide is required
9	Gram stain is not performed. No slide is required.

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 29 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1
Next Review Date: 15/03/2026 Policy Number: 15/03/2024

# 16. PROCEDURE INSTRUCTIONS: RESPIRATORY CULTURE

Step	Action
1	<ul> <li>Sputum</li> <li>Endotracheal aspirate</li> <li>Auger suction</li> <li>Bronchial aspirates (washings)</li> <li>Bronchoalveolar lavage (BAL)</li> </ul>
2	Specimen should be refrigerated.
3	<ul> <li>Criteria for rejection:</li> <li>1. Unlabeled/mislabelled specimen</li> <li>2. Specimen container label does not match patient identification on requisition</li> <li>3. Swabs of sputa</li> <li>4. Duplicate specimens obtained with the same collection method within 24 hours</li> <li>5. Leaking specimens</li> <li>7. Improperly collected, labeled, transported or handled bronchial aspirate (wash specimens), BAL specimens, lung aspirates and lung biopsy specimens should be processed. Waiver of responsibility form SCM40110 needs to be filled out by the responsible nurse</li> </ul>
4	<ul> <li>Label the following media/slides:</li> <li>BA-C: Blood agar</li> <li>CHO-C: Chocolate agar</li> <li>MAC-O: MacConkey agar</li> <li>Label the frosted end of a glass microscope slide with accession number, patient's last name and specimen type</li> </ul>
5	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.
6	Make Gram stain smear. Refer to MIC10000-Microbiology Specimen Handling.
7	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.
8	Place MAC plate in the O₂ incubator on "New Respiratory Culture" shelf.
9	Place BA and CHO plates in the CO <sub>2</sub> incubator on "New Respiratory Culture" shelf.
10	Gram stain slide. Refer to MIC20100-Gram Stain.

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 30 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1
Next Review Date: 15/03/2026 Date Approved: 15/03/2024

17. PROCEDURE INSTRUCTIONS: THROAT CULTURE

	COLLONE INSTRUCTIONS. TIROAT COLLONE
Step	Action
1	Throat swab
2	Specimen should be stored at room temperature.
3	<ul> <li>Criteria for rejection:</li> <li>1. Unlabeled/mislabelled specimen</li> <li>2. Specimen container label does not match patient identification on requisition</li> <li>3. Duplicate specimens obtained with same collection method within 24 hours</li> </ul>
4	<u>Label the following media/slides</u> :  • BA-2: Blood agar
5	Inoculate plate with specimen. Refer to MIC10000-Microbiology Specimen Handling.
6	Streak plate for isolation. Refer to MIC10000-Microbiology Specimen Handling.
7	Place BA plate in "For throat jar" rack in the CO <sub>2</sub> incubator.
8	Gram stain is not performed. No slide is required.

# 18. PROCEDURE INSTRUCTIONS: TIP CULTURE

Step	Action
1	<ul> <li>Intravascular catheters including: central, CVC, peripheral, arterial, jugular, femoral, subclavian, umbilical, hyperalimentation, hemodialysis, port-a-cath and swan-Ganz</li> </ul>
2	Specimen should be refrigerated.
3	<ul> <li>Criteria for rejection:</li> <li>1. Unlabeled/mislabelled specimen</li> <li>2. Specimen container label does not match patient identification on requisition</li> <li>3. Foley catheter tips are not acceptable for culture</li> <li>4. Chest tube tips and abdominal drain tips</li> <li>5. Catheter tips should not be placed in saline or transport medium</li> </ul>
4	<ul><li>Label the following media/slides:</li><li>BA-C: Blood agar</li><li>MAC-O: MacConkey agar</li></ul>
5	Using a sterile needle or loop, roll the segment back and forth 4 times across the surface of the Blood agar plate followed by the MacConkey plate.  NOTE: If the tip is too long, cut the proximal end with sterilized scissors prior to rolling onto plates
6	Place MAC plate in the O <sub>2</sub> incubator on "New Wound Culture" shelf.
7	Place BA plate in the CO <sub>2</sub> incubator on "New Wound Culture" shelf.
8	Gram stain is not performed. No slide is required.

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 31 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1

Next Review Date: 15/03/2026

Date Approved: 15/03/2024

19. PROCEDURE INSTRUCTIONS: Toxigenic C.difficile

Step		Action		
1	•	Refer to MIC10300-Xpert <i>C.difficile</i>		

20. PROCEDURE INSTRUCTIONS: Trichomonas Rapid Test

Step		Action
1	•	Refer to MIC10350-OSOM <i>Trichomonas</i> Rapid Test

#### 21. PROCEDURE INSTRUCTIONS: URINE CULTURE

<u>21. P</u>	ROCEDURE INSTRUCTIONS: URINE CULTURE			
Step	Action			
NOTE	Due to incubation requirements, urine plates are set up until 15:00			
1	<ul> <li>Fresh urine collected in sterile container</li> <li>Fresh urine collected in urine transport tube</li> </ul>			
2	<ul> <li>Urine in sterile container should be refrigerated</li> <li>Urine in urine transport tube can be kept at room temperature or refrigerated</li> </ul>			
3	<ul> <li>Criteria for rejection:</li> <li>1. Unlabeled/mislabelled specimen</li> <li>2. Specimen container label does not match patient identification on requisition</li> <li>3. Duplicate specimens obtained with the same collection method within 24 hours</li> <li>4. Refrigerated fresh urine specimens received &gt;24 hours after collection</li> <li>5. 24-hour urine collections</li> <li>6. Foley catheter tips</li> <li>7. Specimens in leaking container</li> </ul>			
<b>4 5</b>	Label the following media/slides:  • UR1-O: UriSelect 4 agar for non-sterile urine specimens  • UR2-O: UriSelect 4 agar for sterile urine specimens  NOTE: Highlight urine type on plate if UR2-O  Inoculate plate with specimen. Refer to MIC10000-Microbiology Specimen Handling.			
6	Streak plate for isolation. Refer to MIC10000-Microbiology Specimen Handling.			
7	Place URI plate in the O₂ incubator on "New Urine Culture" shelf.			

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 32 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

#### 22. PROCEDURE INSTRUCTIONS: VRE SCREEN

Step	Action		
NOTE	Due to incubation requirements, VRE plates are set up until 15:00		
1	<ul><li>Swab specimen</li><li>Stool specimens</li></ul>		
2	Specimen should be stored at room temperature.		
3	<ul> <li>Criteria for rejection:</li> <li>1. Unlabeled/mislabelled specimen</li> <li>2. Specimen container label does not match patient identification on requisition</li> <li>3. Duplicate specimens obtained with same collection method from same collection location within 24 hours</li> <li>4. Nasal and axilla swabs should not be processed for VRE</li> <li>Label the following media/slides:</li> <li>VRE-O: VRESelect agar</li> </ul>		
5	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.		
6	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.		
7	Label the VRE plate with: R: (Date + 1 date + 2 date) and time incubated.		
8	Place VRE plate in the O <sub>2</sub> incubator on "New Urine Culture" shelf.		

#### 23. PROCEDURE INSTRUCTIONS: WET PREP SCREEN

Step	Action		
NOTE	NOTE: Wet prep is only performed in absence of Trichomonas Rapid Test		
1	<ul><li>Cervix</li><li>Urethra (male)</li><li>Vagina</li></ul>		
2	Specimen should be stored at room temperature.		
3	<ol> <li>Criteria for rejection:         <ol> <li>Specimen is &gt;72 hours old</li> <li>Unlabeled/mislabelled specimen</li> <li>Specimen container label does not match patient identification on requisition</li> </ol> </li> <li>Duplicate specimens obtained with same collection method within 24 hours</li> </ol>		
4	<u>Label the following media/slides</u> : • WPGS: Glass test tube		
5	Place labeled glass test tube into a rack and add approximately 0.5 mL of saline.		
6	Place the culture swab into the saline and mix. Place the swab transport tube in the slot behind the glass test tube.		
7	Incubate in the $O_2$ incubator for at least 15 minutes.		

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Page 33 of 37 Date Approved:

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1

Next Review Date: 15/03/2026

Policy Number: 15-03/2024

24. PROCEDURE INSTRUCTIONS: WOUND CULTURE

10

a. S	uperficial Wound			
Step	Action			
1	<ol> <li>Superficial wound specimens:         <ul> <li>Abrasion, cut, laceration, ulcer, skin diseases (impetigo, folliculitis, cellulitis), first degree burn, superficial surgical incision, etc.</li> </ul> </li> <li>Superficial specimens:         <ul> <li>Boils, cyst, etc.</li> </ul> </li> <li>Drain specimens:         <ul> <li>J-tubes, G-tubes, chest tube, abdominal, etc.</li> </ul> </li> </ol>			
2	Specimen should be stored at room temperature.			
3	<ol> <li>Criteria for rejection:</li> <li>Unlabeled/mislabelled specimen</li> <li>Specimen container label does not match patient identification on requisition</li> <li>Specimens for culture submitted in container with formalin.</li> <li>Submission of specimens to determine <i>if</i> an infection is present should be discouraged</li> </ol>			
4	<ul> <li>Label the following media/slides:</li> <li>BA-C: Blood agar</li> <li>CNA-C: Colistin-nalidixic acid agar</li> <li>MAC-O: MacConkey agar</li> <li>Label the frosted end of a glass microscope slide with accession number, patient's last name and specimen type</li> </ul>			
5	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.			
6	Make Gram stain smear. Refer to MIC10000-Microbiology Specimen Handling.			
7	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.			
8	Place BA and CNA plates in the CO <sub>2</sub> incubator on "New Wound Culture" shelf.			
9	Place MAC plate in the O <sub>2</sub> incubator on "New Wound Culture" shelf.			

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Gram stain slide. Refer to MIC20100-Gram Stain.

Policy Number: Date Approved: Page 34 of 37

Type: Laboratory Services Program SOP

Title: MIC10100-Microbiology Specimen Processing Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

b. Deep Wound

Step	Action			
Step				
1	<ul><li>Swab</li><li>Aspirate/drainage/pus received in sterile container</li></ul>			
2	Specimen should be stored at room temperature.			
3	<ul> <li>Criteria for rejection:</li> <li>1. Unlabeled/mislabelled specimen</li> <li>2. Specimen container label does not match patient identification on requisition</li> <li>3. Specimens for culture submitted in container with formalin</li> </ul>			
4	<ul> <li>Label the following media/slides:</li> <li>BA-C: Blood agar</li> <li>CHO-C: Chocolate agar</li> <li>CNA-C: Colistin-nalidixic acid agar</li> <li>MAC-O: MacConkey agar</li> <li>BRU-2: Brucella agar</li> <li>KV-2: Anaerobic KV agar</li> <li>Label the frosted end of a glass microscope slide with the accession number, patient's last name and specimen type</li> </ul>			
5	Inoculate plates with specimen. Refer to MIC10000-Microbiology Specimen Handling.			
6	Make Gram stain smear. Refer to MIC10000-Microbiology Specimen Handling.			
7	Streak plates for isolation. Refer to MIC10000-Microbiology Specimen Handling.			
8	Place MAC plate in the O <sub>2</sub> incubator on "New Wound Culture" shelf.			
9	Place BA and CHO plates in the CO <sub>2</sub> incubator on "New Wound Culture" shelf.			
10	Place BRU and KV in anaerobic jar or tray with anaerobic pouch and indicator as soon as practical after inoculation. Label jar or tray with date of 48 hour read. Anaerobes should not be exposed to air for 42-48 hours after inoculation. Refer to MIC10000-Microbiology Specimen Handling.			
11	Gram stain slide. Refer to MIC20100-Gram Stain.			

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 35 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services Policy Number: 15-146-V1
Next Review Date: 15/03/2026 Date Approved: 15/03/2024

25. PROCEDURE INSTRUCTIONS: YEAST CULTURE

Step	Action		
1	<ul> <li>Anal</li> <li>Cervix</li> <li>Penis</li> <li>Vagina</li> <li>NOTE: Refer to MIC10110-Vaginal Swab Processing Job Aid for yeast culture ordered on vaginal swabs</li> </ul>		
2	Specimen should be stored at room temperature.		
3	<ul><li>Criteria for rejection:</li><li>1. Unlabeled/mislabelled specimen</li><li>2. Specimen container label does not match patient identification on requisition</li></ul>		
4	Label the following media/slides:  SAB-R: Sabouraud dextrose agar		
5	Inoculate plate with specimen. Refer to MIC10000-Microbiology Specimen Handling.		
6	Streak plate for isolation. Refer to MIC10000-Microbiology Specimen Handling.		
7	Label SAB plate with R: (Date + 2 date).		
8	Place SAB plate on urine bench and "incubate" at room temperature.		
9	Gram stain is not performed. No slide is required.		

#### **CROSS-REFERENCES:**

- MIC10000-Microbiology Specimen Handling
- MIC10110-Vaginal Swab Processing Job Aid
- MIC10300-Xpert C.difficile
- MIC10350-OSOM Trichomonas Rapid Test
- MIC20100-Gram Stain
- MIC60010-Microbiology Quality Control procedure
- MIC60040-Culture Media Quality Control procedure
- MIC71000-BACTEC FX Instrument
- SCM40100-Specimen Acceptance and Rejection Policy
- SCM40110-Waiver of Responsibility Form

#### **REFERENCES:**

- Leber, A. (2016). Clinical microbiology procedures handbook. (4<sup>th</sup>ed.) Washington, D.C.: ASM Press
- Jorgensen J.H., Pfaller M.A., Carroll K.C., Funke G., Landry M.L., Richter S.S., Warnock D.W. (2015). *Manual of Clinical Microbiology*, 11<sup>th</sup> edition. Washington, D.C: ASM Press

**Disclaimer Message:** This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Date Approved: Page 36 of 37

Issuing Authority: Director, Laboratory and Diagnostic Imaging Services

Policy Number: 15-146-V1 Next Review Date: 15/03/2026 Date Approved: 15/03/2024

# **APPROVAL:**

March 15, 2024

Date

Director, Laboratory and Diagnostic Imaging Services

# **REVISION HISTORY:**

REVISION	DATE	Description of Change	REQUESTED BY
1.0	11 Aug 2016	Initial Release	L. Steven
2.0	10 Jun 2019	Update to reflect new urine chromogenic agar	L. Steven
3.0	27 Feb 2020	Procedure reviewed	L. Steven
4.0	30 Jan 2022	Procedure reviewed and added to NTHSSA policy template	L. Steven
5.0	14 Feb 2024	Procedure reviewed	L. Steven

Disclaimer Message: This is a CONTROLLED document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Policy Number: Page 37 of 37 Date Approved: