

PROGRAM Standard Operating Procedure – Laboratory Services	
Title: MIC10300 – Xpert <i>C.difficile</i>	Policy Number: 15-148-V1
Program Name: Laboratory Services	
Applicable Domain: Lab, DI and Pharmacy Services	
Additional Domain(s): NA	
Effective Date: 18/03/2024	Next Review Date: 18/03/2026
Issuing Authority: Director, Laboratory and Diagnostic Imaging Services	Date Approved: 18/03/2024
Accreditation Canada Applicable Standard: NA	

Uncontrolled When Printed

GUIDING PRINCIPLE:

The Xpert *C.difficile* assay is a qualitative *in vitro* diagnostic test for rapid detection of toxin B gene sequences from unformed (liquid or soft) stool specimens collected from patients suspected of having *Clostridium difficile* infection (CDI). The test utilizes automated real time polymerase chain reaction (PCR) to detect toxin gene sequences associated with toxin producing *C.difficile*.

PURPOSE/RATIONALE:

This standard operating procedure describes the Xpert *C.difficile* test using the GeneXpert Dx System.

SCOPE/APPLICABILITY:

This standard operating procedure applies to Medical Laboratory Technologists (MLTs) processing specimens for *C.difficile* using the GeneXpert Dx System.

SAMPLE INFORMATION:

Type	Stool (Unformed)
Collection Container	<ul style="list-style-type: none"> Orange top, sterile container
Stability	<ul style="list-style-type: none"> Room temperature up to 24 hours Refrigerated up to 5 days
Storage Requirements	Room temperature or refrigerated
Criteria for rejection	<ol style="list-style-type: none"> Unlabeled/mislabeled samples Sample container label does not match patient identification on requisition Sample not in sterile container

Disclaimer Message: This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

4. Sample not stored correctly
5. Repeat testing on positive samples will not be performed within 7 days (Cancellation code: |XCDP)
6. Repeat testing on negative samples will not be performed within 7 days (Cancellation code: IXCDN)
7. Testing will not be performed on patients <12months old (Cancellation code: |XCD1)
8. Testing for *C. difficile* Toxin is not performed on formed stools (Cancellation code: IXCDT)

REAGENTS and/or MEDIA:

- Xpert *C.difficile* cartridge
- Sample reagent

SUPPLIES:

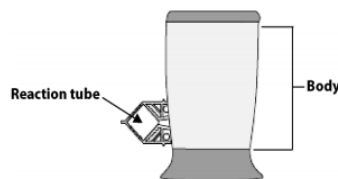
- Personal protective equipment
- Dry waste container
- Sterile, dry swabs
- Disposable transfer pipettes

EQUIPMENT:

- GeneXpert Dx System
- Printer
- Class II biosafety cabinet (BSC)
- Vortex mixer
- Refrigerator

ENVIRONMENTAL CONTROLS:

- Store Xpert *C.difficile* cartridges upright between 2°C to 28°C
- Do not use a cartridge that has been damaged or leaked, dropped, or shaken
- Open a cartridge only when ready to add sample. An open cartridge must be loaded onto the GeneXpert within 30 minutes
- Cartridges are single use. Do not attempt to open or re-use a cartridge
- Cartridges and test samples stored at 4°C must be brought to room temperature before running the assay
- Do not touch the Reaction Tube, always handle the cartridge by its Body



SPECIAL SAFETY PRECAUTIONS:

Containment Level 2 facilities, equipment, and operational practices for work involving infectious or potentially infectious materials or cultures:

- Ensure that appropriate hand hygiene practices be used
- Lab gown must be worn when performing activities with potential pathogens
- Gloves must be worn when direct skin contact with infected materials is unavoidable
- Eye protection must be used when there is a known or potential risk of exposure of splashes
- All procedures that may produce aerosols, or involve high concentrations or large volumes should be conducted in a biological safety cabinet (BSC)
- The use of needles, syringes and other sharp objects should be strictly limited

All patient specimens are assumed to be potentially infectious. Routine Practices must be followed. Since viable micro-organisms are used, all cultures must be handled with appropriate precautions. All equipment in contact with cultures should be decontaminated by appropriate methods.

QUALITY CONTROL:

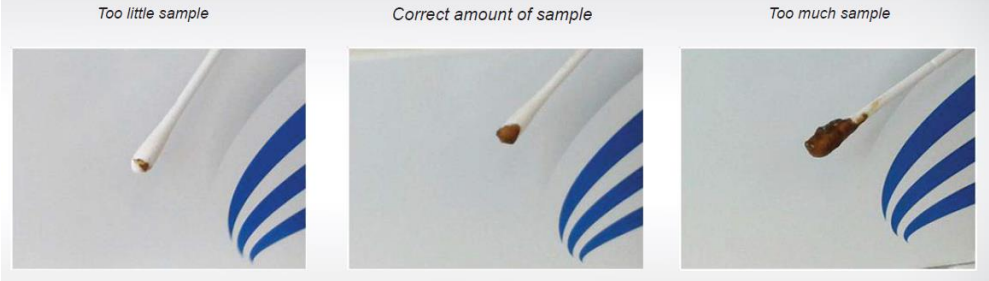

- Refer to MIC60080-Xpert *C.difficile* Quality Control for quality control procedure
- Record all results on MIC60081-QC Results Record-Xpert *C.difficile*

PROCEDURE INSTRUCTIONS:

Step	Action
Preparing the Run	
1	Order GeneXpert <i>C.difficile</i> testing in the LIS: <ul style="list-style-type: none"> • Medipatient the order if required • In SoftMic, accession the order using the test code PCCDI • Add any "copies to" if required • Collect, receive and plate the order • Label the requisition with the requisition label and scan into SoftMedia • Place the sample barcode label on the sample and the barcode label in the pouch of the biohazard bag for when the sample is being processed
2	Ensure the daily maintenance for the GeneXpert has been completed and is documented on MIC72110-Maintenance Record-GeneXpert.

Step	Action
Preparing the Cartridge	
1	Remove the cartridge and reagent from the package. Acquire a swab and a pipette for each sample being tested.
2	Apply the media barcode label to the right hand side of the cartridge, near the base. NOTE: Do not cover the barcode label on the front of the cartridge

Disclaimer Message: This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

3	The test must be started within 30 minutes of adding reagents to the cartridge.
4	Vortex the sample for 10 seconds to ensure it is evenly mixed.
5	Briefly place a swab in the unformed stool sample. The swab does not need to be completely saturated: 
6	Insert the swab into the vial containing the Sample Reagent.
7	Hold the swab by the stem near the rim of the vial and push the stem against the edge of the vial to break it. NOTE: Make sure the swab is short enough to allow the cap to close
8	Close the lid and vortex at high speed for 10 seconds.
9	Pry open the cartridge lid and open wrapper of the transfer pipette.
10	Transfer the entire contents of the Sample Reagent to the Sample Chamber of the cartridge: 
11	Firmly snap close the lid to seal the cartridge and place in the cartridge tray.

Step	Action
Creating a Test Run	
1	Transfer the loaded cartridges in the cartridge tray to the GeneXpert bench.
2	Log into the GeneXpert software using the username admin1 and the password covid19 .
3	Confirm that all modules are detected by the software and ready for testing.
4	On the GeneXpert software, click Create Test at the top left.
5	Using the scanner, scan the sample ID barcode and the cartridge barcode. Select Start Test .
6	Locate the module with the blinking green light, open the module door and load the cartridge.
7	Close the module door firmly, it will latch closed.

Disclaimer Message: This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

Step	Action
Generating a Test Report	
1	A report is generated automatically upon completion of a run.
2	To view runs or reprint: Select View Results on the menu bar. Click Report → Check Patient ID → Click Preview PDF → Click Print

INTERPRETATION OF RESULTS:

RESULT	INTERPRETATION
NEGATIVE	<ul style="list-style-type: none"> <i>C.difficile</i> target DNA sequences are not detected Toxins producing <i>C.difficile</i> targets not detected
POSITIVE	<ul style="list-style-type: none"> <i>C.difficile</i> target DNA sequences are detected The toxin producing <i>C.difficile</i> target(s) have Cts within the valid range
NO RESULT	<ul style="list-style-type: none"> Presence or absence of <i>C.difficile</i> target DNA cannot be determined
ERROR/INVALID	<ul style="list-style-type: none"> Presence or absence of <i>C.difficile</i> cannot be determined Toxin producing <i>C.difficile</i> targets-NO RESULT Probe Check: FAIL; one or more probe checks have failed

REPORTING INSTRUCTIONS:

Toxigenic <i>C.difficile</i> NEGATIVE	<ul style="list-style-type: none"> Report: NEGATIVE
Toxigenic <i>C.difficile</i> POSITIVE	<ul style="list-style-type: none"> Report: POSITIVE Phone results to patient location <ul style="list-style-type: none"> ➢ Document call in the Call Box in SoftMic Report will automatically print to OCPHO (HPU1) Report will automatically print to Stanton IPAC (SIPAC) and Inuvik IPAC (IIPAC) if ER or inpatient
Toxigenic <i>C.difficile</i> NO RESULT	<ul style="list-style-type: none"> Retest the sample with a new cartridge <ul style="list-style-type: none"> ➢ Add comment in TCOMM that testing was repeated If repeat testing is the same: <ul style="list-style-type: none"> ➢ Phone the ordering location and request a new sample be collected ➢ Report: NO RESULT - Presence of C.diff toxin cannot be determined ➢ From the keypad add key R to add repeat sample collection comment

Disclaimer Message: This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.

LIMITATIONS:

1. This test detects but does not differentiate the NAP1 (Ribotype 027) strain from other toxigenic strains of *C.difficile*.
2. This test targets the *tcdB* gene for Toxin B production. This test will not detect strains of *C.difficile* that do not contain the *tcdB* gene.
3. Positive results observed with immunocompromised pediatric patients may reflect asymptomatic carriage of *C.difficile*.
4. Results from the Xpert *C.difficile* Assay should be interpreted in conjunction with other laboratory and clinical data available to the clinician.
5. Erroneous test results might occur from improper specimen collection, failure to follow the recommended sample collection, handling and storage procedures, technical error, sample mix-up, or because the number of organisms in the specimen is too low to be detected by the test.
6. Inhibition of the Xpert *C.difficile* Assay has been observed in the presence of the following substances: Zinc oxide paste and Vagisil cream.
7. False negative results may occur when the infecting organism has genomic mutations, insertions, deletions or rearrangements or when performed early in the course of illness.

CROSS-REFERENCES:

- MIC60080-Xpert *C.difficile* Quality Control
- MIC60081-QC Results Record-Xpert *C.difficile* QC
- MIC72110-Maintenance Record-GeneXpert

REFERENCES:

1. Cepheid GeneXpert. Xpert *C. difficile* Assay Instructions for Use. 300-9680 Rev. F, March 2016
2. Cepheid GeneXpert. *Dx System User Manual*. 301-0045, Rev.C, June 2012

APPROVAL:

March 18, 2024

Date



Director, Laboratory and Diagnostic Imaging Services

REVISION HISTORY:

REVISION	DATE	Description of Change	REQUESTED BY
1.0	30 Jan 22	Initial Release	L. Steven
2.0	14 Feb 24	Procedure reviewed	L. Steven

Disclaimer Message: This is a **CONTROLLED** document for internal use only. Any documents appearing in paper form are not controlled and should be checked against the electronic file version prior to use.