



University of Washington Medical Center 1959 NE Pacific Street. Seattle, WA 98195 Transfusion Services Laboratory Policies and Procedures Manual	Original Effective Date: 03-27-21	Number: EQ-0013.03
	Revision Effective Date: 04-25-22	
TITLE: HaemoBank and BloodTrack Courier: Operation & Troubleshooting		

PURPOSE:

To provide instructions for troubleshooting problems with the HaemoBank and BloodTrack Courier Kiosk including emergency access to evacuate blood components and perform maintenance

LOCATION:

Northwest Lab Transfusion Support Service (TSS)


PRINCIPLE & CLINICAL SIGNIFICANCE:




NA

POLICIES:

- Evacuation of blood components using the method specified below should only be used when BloodTrack Courier is offline. When BloodTrack Courier is available use the standard bulk move out process outlined in SOP ***Returning Blood Components to Montlake from Northwest Campus***
- For issues with the SATO printer that prints Transfusion Record labels for blood component removed from the HaemoBank refer to SOP ***HaemoBank SATO Printer: Operations and Troubleshooting***

Definitions

Name	Description
HaemoBank	Temperature controlled point-of-care storage device (refrigerator) utilized by NW to store red blood cell components (RBC). RBC are loaded, unloaded, remotely allocated and issued from this device using Blood Track Courier software. 
BloodTrack Courier software	Software that runs on the BloodTrack kiosk which controls access to the HaemoBank. BloodTrack Courier is used to load, unload blood components and issue blood components from the HaemoBank.

Name	Description
<p>BloodTrack Kiosk</p>	<p>A standalone computer system that controls access to the HaemoBank for loading, unloading and issuing blood components. The computer runs on a Microsoft Office operating system and includes an intuitive touchscreen interface on the face of the HaemoBank.</p> <p>NOTE: Does not control refrigeration functionality of the HaemoBank.</p> 
<p>Helmer Refrigerator</p>	<p>The refrigerator portion of the HaemoBank for blood storage. Storage temperature and operational alarms are controlled via the i.C3 Information Center centered directly above the door.</p> 
<p>i.C³ Information Center</p>	<p>The Helmer i.C³ Information Center is integrated into the HaemoBank refrigerator to provide diagnostic information, temperature data and status of the refrigerator. Allows one to monitor and optimize performance of the refrigerator</p> 

REAGENTS/SUPPLIES/EQUIPMENT:

Reagents:	Supplies:	Equipment:
NA	NA	NA

QUALITY CONTROL:

NA

INSTRUCTIONS:



TABLE OF CONTEXT

- [Restarting BloodTrack Courier Software](#)
- [Restarting BloodTrack Kiosk](#)
- [Shutting Down BloodTrack Courier Kiosk](#)
- [Emergency Access for Evacuation of Blood Components](#)
- [Bringing HaemoBank Online After Emergency Access \(Bypass Rest\)](#)
- [Maintenance Access to the HaemoBank](#)

Restarting BloodTrack Courier Software

Use when software is frozen, a tray is disabled, or other software error has occurred.

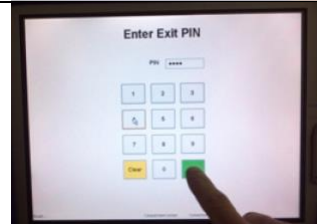
STEP	ACTION	
1	Touch the bottom right area of the BloodTrack Courier screen to access the keyboard as shown in the picture to the right	
	If Unable to exit BloodTrack Courier screen	Then Go to section Shutting Down BloodTrack Courier Kiosk
2	<ul style="list-style-type: none"> Enter exit pin, 1 2 3 4 Touch <Ok> 	
3	Double click on the <BloodTrack Courier> icon on the Windows home screen	
4	If connectivity is Restored	Then No further action is required
	Not restored	Go to next section Restarting BloodTrack Kiosk





Restarting BloodTrack Courier Kiosk

Use when restarting the BloodTrack Courier (instructions above) does not resolve problem.


STEP	ACTION	
1	Touch the bottom right area of the BloodTrack Courier screen to access the keyboard as shown in the picture to the right	
	If Unable to exit BloodTrack Courier screen	Then Go to section Shutting Down BloodTrack Courier Kiosk
2	<ul style="list-style-type: none"> Enter exit pin, 1 2 3 4 Touch <Ok> 	



STEP	ACTION	
3	Select <Window Start Menu> icon	
4	Press the arrow and press the "Restart" on the pop-up window to restart NOTE: The HaemoBank and BloodTrack courier will both reinitialize	
5	If connectivity is	Then
	Restored	No further action is required
	Not restored	Go to next section Shutting Down BloodTrack Courier Kiosk





Shutting Down BloodTrack Courier Kiosk

Perform when BloodTrack courier is frozen and unable to restart. Consult with TSS supervisor or Lead prior to performing the following steps.

STEP	ACTION	
1	Locate the black " ON/OFF " button on the access console on top of the HaemoBank, above the PC monitor towards the back of the device. The button can be found just below the blue power cord plug.	
2	<ul style="list-style-type: none"> • Push the power button once to shut the PC down • Allow the PC to shut down completely 	
3	Push the power button again to power on and restart the PC	
	If PC	Then
	Powers on and restart	<ul style="list-style-type: none"> • PC will power on and restart • BloodTrack courier will automatically reinitialized
	Still frozen	Unplug the power cord for the PC <ul style="list-style-type: none"> • Locate the cord for the PC on top of the HaemoBank. • Press down on the yellow button and turn the cord to unplug • Wait 20 seconds before plugging the PC back in
4	If connectivity is	Then
	Restored	No further action is required
	Not restored	Contact Haemonetics technical support line

Emergency Access for Evacuation of Blood Components

Perform to evacuate blood components during unplanned downtime due to refrigeration or power failure.

STEP	ACTION
1	Call the ML TSL to let them know blood components are being evacuated due to temperature or power failure.
2	Locate the Helmer iC ³ user interface on the front of the HaemoBank device above the main door
3	Touch the APPS icon  on the bottom left side of the screen to view the iC ³ applications
4	<ul style="list-style-type: none"> • Scroll to the right and locate the lock padlock icon • Touch the locked padlock icon  on the screen
5	Access control screen will display a keypad for accessing the device door
6	Enter the passcode 9972 when prompted
7	Padlock icon will display unlocked and an audible click will be heard
8	Open the main door
9	<p>Unlock the emergency bypass handle with the “Bypass Handle” key from the key hook on the inside of the storage compartment below the printer drawer.</p> <p>NOTE: The HaemoBank will now be offline. Contact NW or TSL lead or supervisor to bring online.</p>
10	<p>Rotate the bypass release handle counterclockwise to a vertical position to release the locking mechanism for all trays</p> 
11	Pull out the trays and remove all blood components
12	Rotate the emergency bypass handle clockwise to secure the locking mechanism for all trays
13	<ul style="list-style-type: none"> • Lock the emergency bypass handle • Remove the compartment assembly key
14	<p>Close the main door</p> <p>NOTE: Main door will lock</p>
15	Place all blood components in monitored back up refrigerator
16	<p>Print current inventory list from BloodTrack manager</p> <ul style="list-style-type: none"> • Log into ‘BloodTrack Manager’ • Right click on< HaemoBank Refrigerator> • Select <Inventory List> • Click <Print to print inventory li 

STEP	ACTION
17	<p>Update the status of each blood component to 'Out' in BloodTrack Manager unit status to "Out" for each blood component removed from the HaemoBank</p> <ul style="list-style-type: none"> • Click on <Transactions> • Login • Select "Update Unit" • Scan or enter component ID number • Select <Out > form the 'State" dropdown box • Click <Update> at bottom of screen • Repeat for all components removed
18	Return key to designated storage location


Bringing HaemoBank Online After Emergency Access (Bypass Rest)

To be performed by supervisor or lead only (or with approval) after the HaemoBank is confirmed to be acceptable for the storage of blood components and operational for patient use.

STEP	ACTION
1	Confirm that the bypass handle is locked
2	Hold your finger in the top right area of the BloodTrack Courier screen for atleast two seconds to access the BloodTrack Courier Configuration Screen
3	Enter the passcode 19651955 when prompted
4	Touch the <Door Lock Test> button
5	Touch the <Reset Bypass> button
6	Touch the <Done> button
7	Touch the <Cancel> button to return to the main screen

Maintenance Access to the HaemoBank

When access to the refrigerator is needed for annual maintenance and TempTrak probe calibration

STEP	ACTION
1	<p>Open the HaemoBank door to access the chamber temperature probe</p> <ul style="list-style-type: none"> • Touch Home, i.C³ APPS, • Touch Padlock icon  <p>Access Control</p> <ul style="list-style-type: none"> • Enter password 9972 • Door unlocks

**TITLE: HaemoBank and BloodTrack Courier: Operation
& Troubleshooting**

**Number:
EQ-0013.03**

**CALCULATIONS/INTERPRETATIONS/RESULTS REPORTING/NORMAL
VALUES/CRITICAL VALUES**
NA

PROCEDURE NOTES AND LIMITATIONS:

Haemonetics Technical Support Line 1-800-743-5637

REFERENCES:

BloodTrack Courier Manual

RELATED DOCUMENTS:

SOP *Returning Blood Components to Montlake from Northwest Campus*

SOP *HaemoBank SATO Printer: Operations and Troubleshooting*

SOP *Computer and Network Downtime at Northwest Campus*

UWMC SOP Approval:	
UWMC CLIA Medical Director	_____ Date _____
	Andrew Bryan, MD
Transfusion Service Manager	_____ Date _____
	Nina Sen
QA Manager	_____ Date _____
	Tayler Reeves
Transfusion Service Medical Director	_____ Date _____
	Monica Pagano, MD
UWMC Biennial Review:	
	_____ Date _____
	_____ Date _____

REVISION

05/13/2021: Added an additional option when the Kiosk PC cannot be rebooted with the power button
 4/19/2022: Step 2 updated in section Bringing Haemobank Online After Emergency Access updated