

Sample Result Report

11/15/2018 14:13:24

Omaha VA Medical Center
4101 Woolworth Avenue
Omaha, NE 68105
ACL TOP 500 #1
S/N 16053379

Sample ID: ██████████ First Name: ██████████ Rack ID: 04
Sample Type: STAT 0048 Last Name: ██████████ Position ID: 4

Test Code	Results	Type	Rerun	Rerun Needed	Flag	Completed Date & Time	Validated
APTT-SS	19.5 s				LH	10/30/2018 15:39:19	Failed
PT-RP	12.0 s				MT	10/30/2018 15:36:45	Validated
	1.0 INR						

Sample Result Detailed Report

11/15/2018 14:12:51

Omaha VA Medical Center
4101 Woolworth Avenue
Omaha, NE 68105
ACL TOP 500 #1
S/N 16053379


Test Code:	APTT-SS	Test Type:	Patient	Rack ID:	08
Sample ID:	████████0048	Sample Type:	STAT	Position ID:	1

Completed Date & Time: 10/30/2018 15:39:19

	Replicate 1	Replicate 2	Mean
Measured	s 19.5		19.5
	s 19.5		19.5

Replicate 1

Display derivative curves 523.870 1st der 2085.765 2nd der + -840.928 2nd der -

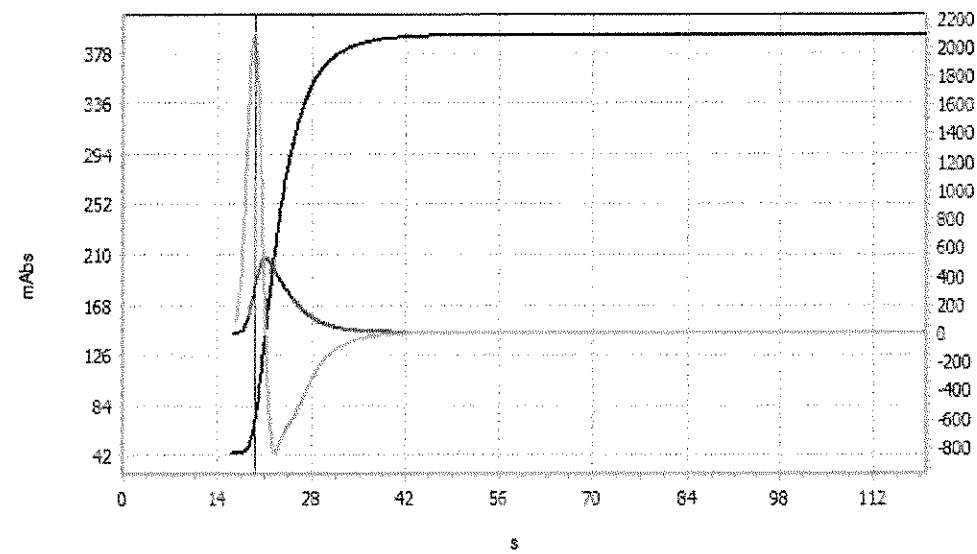

Errors and warnings

- General
- MT 5600 Maintenance overdue or failed
- Replicate 1
- Measured (s)
- LH 5505 Below Therapeutic Range
- Unit 1 (s)
- LH 5505 Below Therapeutic Range

Tracking Information

Material Name	Lot Number	Expiration Date
APTT-SS	N0278340	02/28/2019
APTT-SS CaCl2	N0278349	02/29/2020

User name: top500

Validation Information

Validation Status: Failed