

Sample Result Detailed Report

08/31/2020 11:03:45

Model	ACL TOP 300 CTS	The Heart Hospital Baylor	L. Winneberger, MD
Serial	14011078	1100 Allied Dr	Medical Director
		Plano, Texas 75093	
Test Code:	APTT-SS	Test Type:	Extended(E)
Sample ID:	10054824034	Sample Type:	Patient
		Rack ID:	03
		Position ID:	6


Completed Date & Time: 08/31/2020 08:52:51

	Replicate 1	Replicate 2	Mean
Measured	s FAILED		FAILED
	s FAILED		FAILED

Example 1

Replicate 1

☒ Display derivative curves

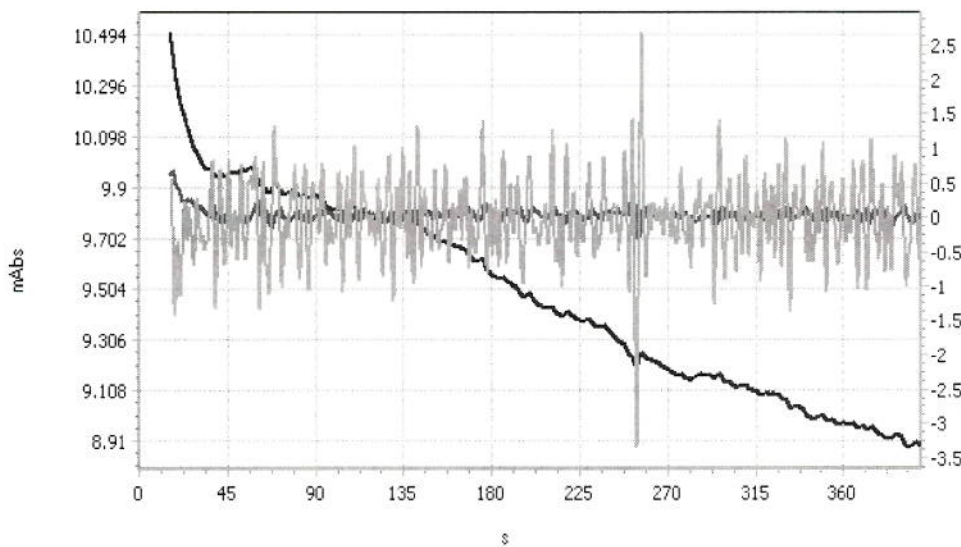

Errors and warnings

		Replicate 1
		Measured (s)
CE	5057	(Data) Curve min. and max. not in correct sequence
		Unit 1 (s)
RE	5100	Measured result failed

Tracking Information

Material Name	Lot Number	Expiration Date
APTT-SS	N0696320	06/30/2021
APTT-SS CaCl2	N0596194	05/31/2022

User name: coagtech
Trigger completed date/time: 08/31/2020 08:42:29

Validation Information

Validation Status: Failed