



Probe with gel

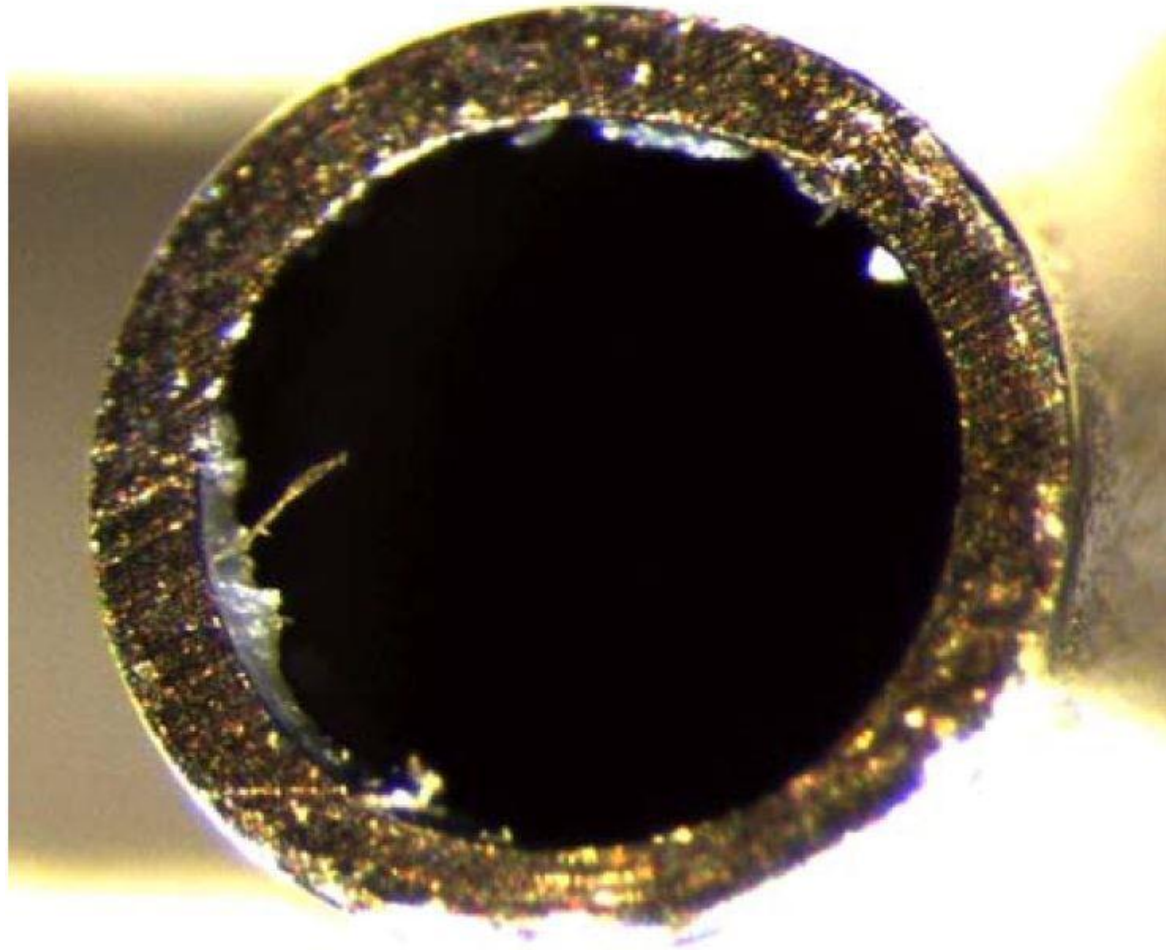

drain with gel

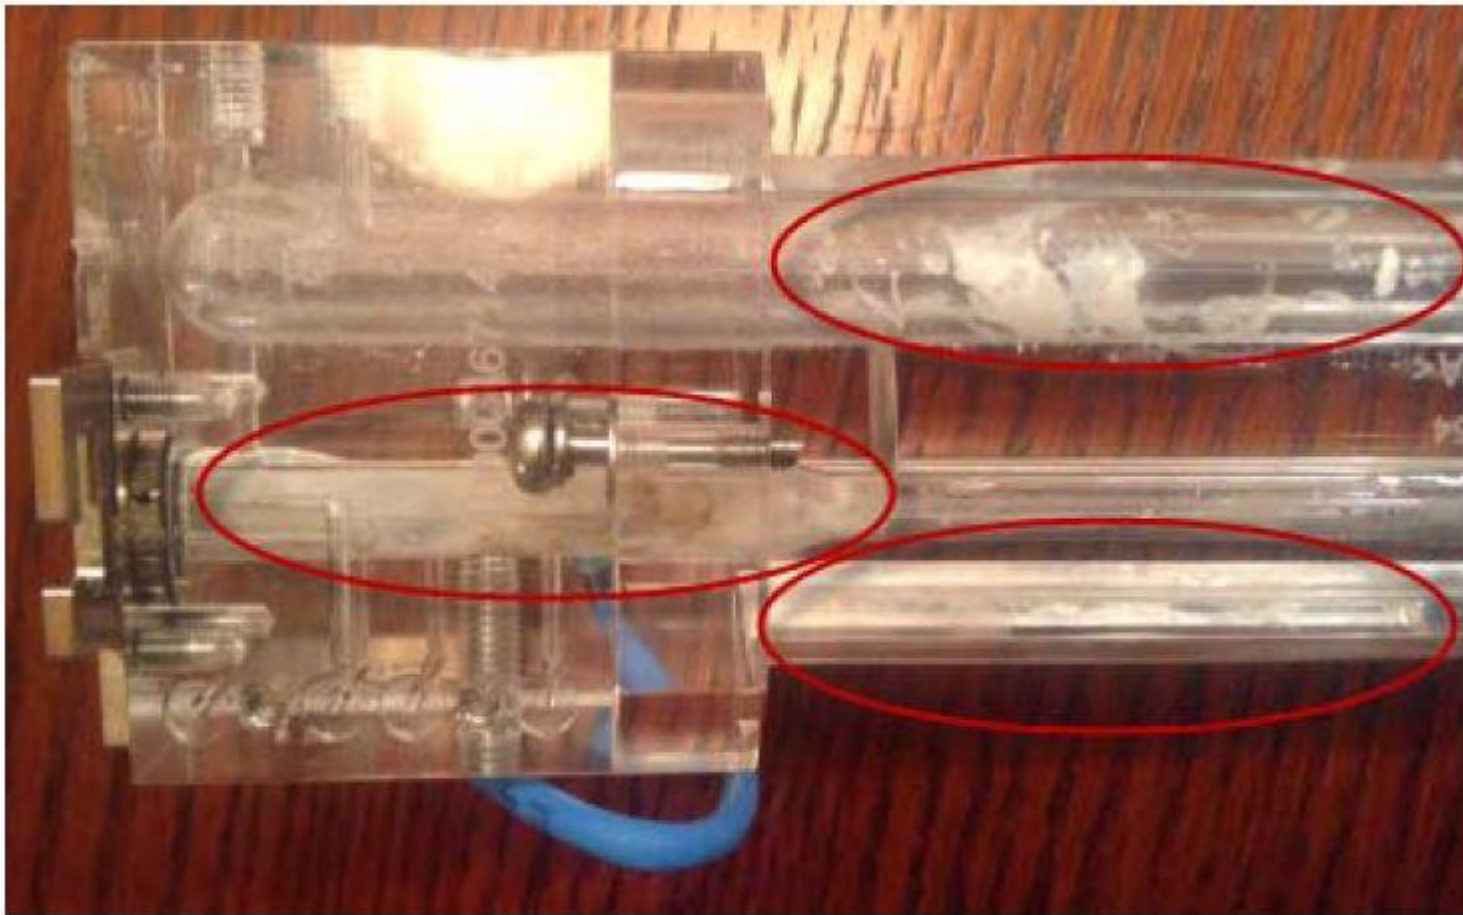

Cellular Debris in Aliquot plate

- It is not always obvious when sample quality is an issue, the inspection of used Vista aliquot plates

CO

